


EZO-ORPTM

Embedded ORP Circuit

Reads	ORP
Range	-1019.9mV – 1019.9mV
Accuracy	+/- 1mV
Max rate	1 reading per sec
Supported probes	Any type & brand
Calibration	Single point
Temp compensation	N/A
Data protocol	UART & I²C
Default I ² C address	98 (0x62)
Operating voltage	3.3V – 5V
Data format	ASCII

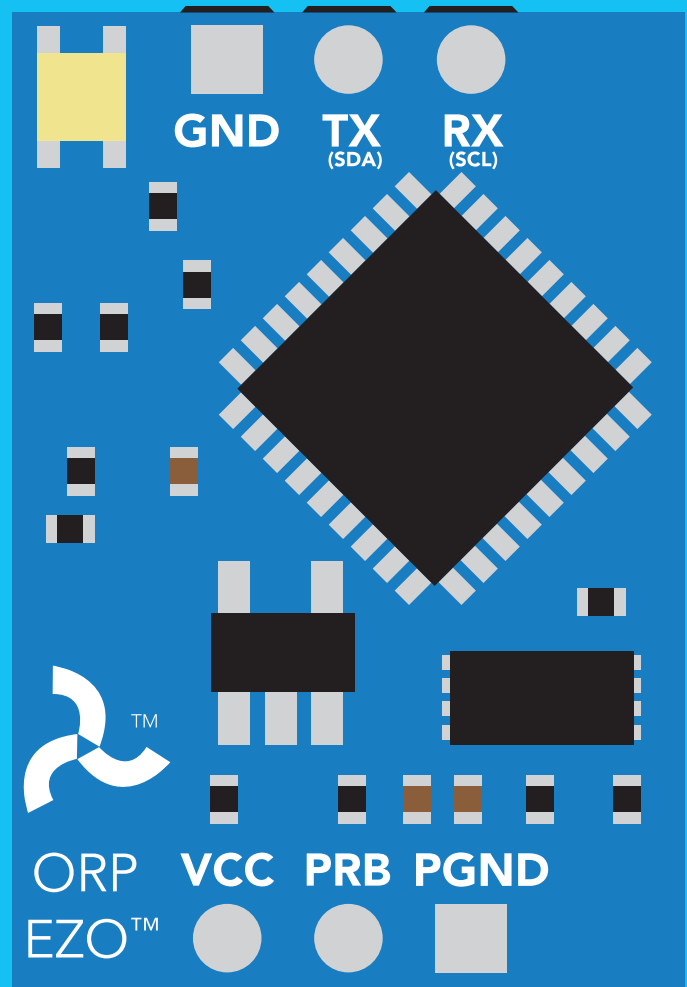

PATENT PROTECTED




STOP

SOLDERING THIS DEVICE VOIDS YOUR WARRANTY.

This is sensitive electronic equipment. Get this device working in a solderless breadboard first. Once this device has been soldered it is no longer covered by our warranty.

This device has been designed to be soldered and can be soldered at any time. Once that decision has been made, Atlas Scientific no longer assumes responsibility for the device's continued operation. The embedded systems engineer is now the responsible party.

Get this device working in a solderless breadboard first!

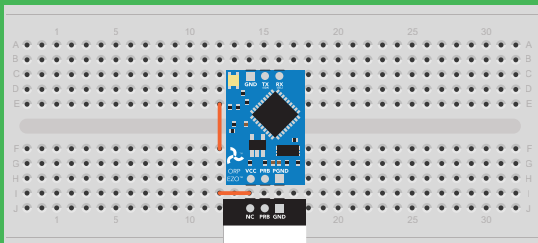

Do not embed this device without testing it in a solderless breadboard!

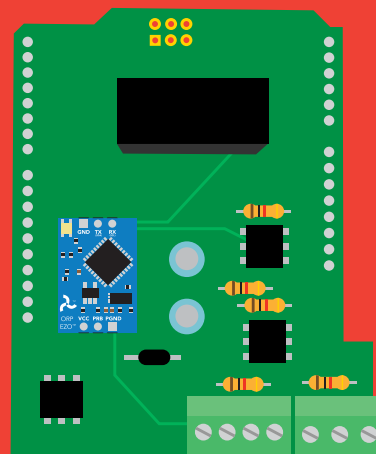


Table of contents

Circuit dimensions	4	Calibration theory	8
Power consumption	4	Power and data isolation	9
Absolute max ratings	4	Correct wiring	11
EZO™ circuit identification	5	Available data protocols	14
Operating principle	6		

UART


UART mode	16
Default state	17
Receiving data from device	18
Sending commands to device	19
LED color definition	20
UART quick command page	21
LED control	22
Find	23
Continuous reading mode	24
Single reading mode	25
Calibration	26
Export/import calibration	27
Naming device	28
Device information	29
Response codes	30
Reading device status	31
Sleep mode/low power	32
Change baud rate	33
Protocol lock	34
Factory reset	35
Change to I ² C mode	36
Manual switching to I ² C	37

I²C

I ² C mode	39
Sending commands	40
Requesting data	41
Response codes	42
LED color definition	43
I²C quick command page	44
LED control	45
Find	46
Taking reading	47
Calibration	48
Export/import calibration	49
Device information	50
Reading device status	51
Sleep mode/low power	52
Protocol lock	53
I ² C address change	54
Factory reset	55
Change to UART mode	56
Manual switching to UART	57

Circuit footprint	58
Datasheet change log	59
Warranty	61

EZO™ circuit dimensions

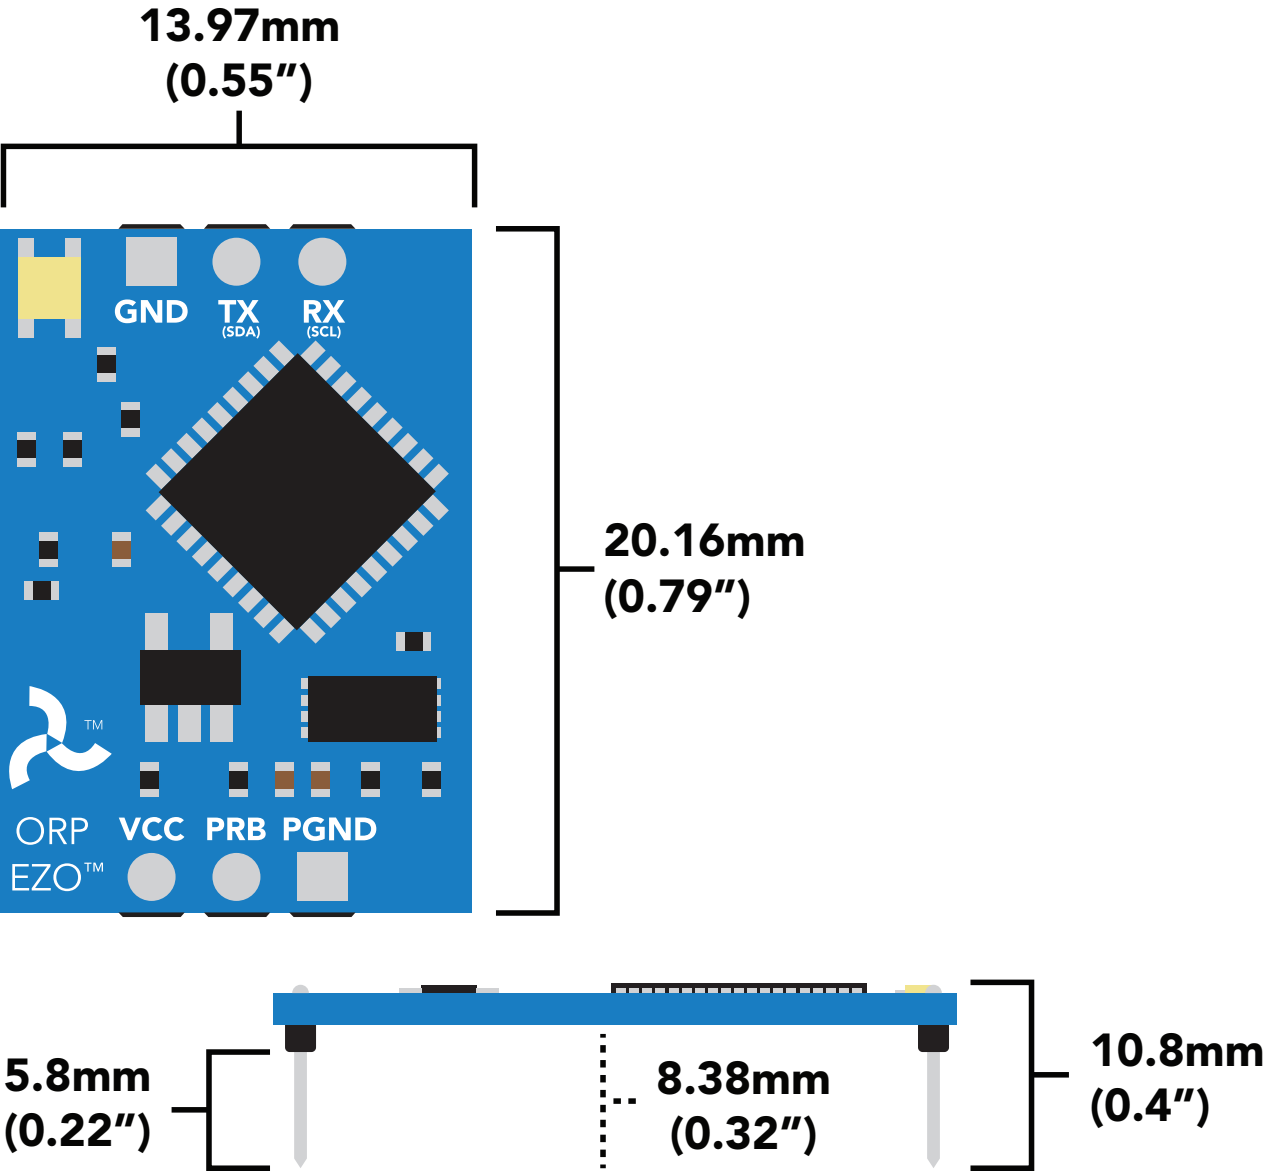


Power consumption

	LED	MAX	STANDBY	SLEEP
5V	ON	18.3 mA	16 mA	1.16 mA
	OFF	13.8 mA	13.8 mA	
3.3V	ON	14.5 mA	13.9 mA	0.995 mA
	OFF	13.3 mA	13.3 mA	

Absolute max ratings

Parameter	MIN	TYP	MAX
Storage temperature (EZO™ ORP)	-65 °C		125 °C
Operational temperature (EZO™ ORP)	-40 °C	25 °C	85 °C
VCC	3.3V	5V	5.5V


EZO™ circuit identification

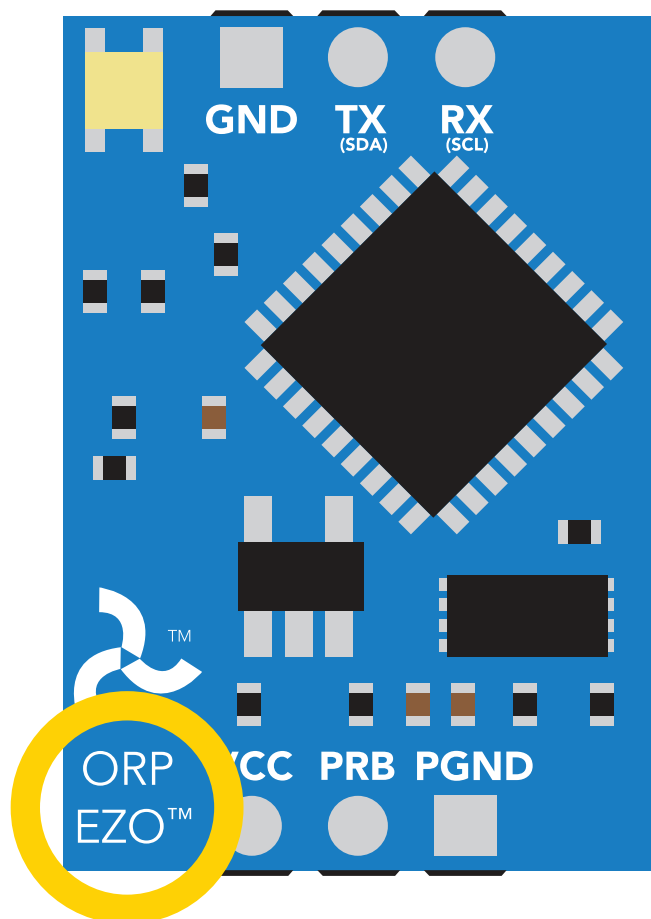

EZO™ ORP circuit



Viewing correct datasheet

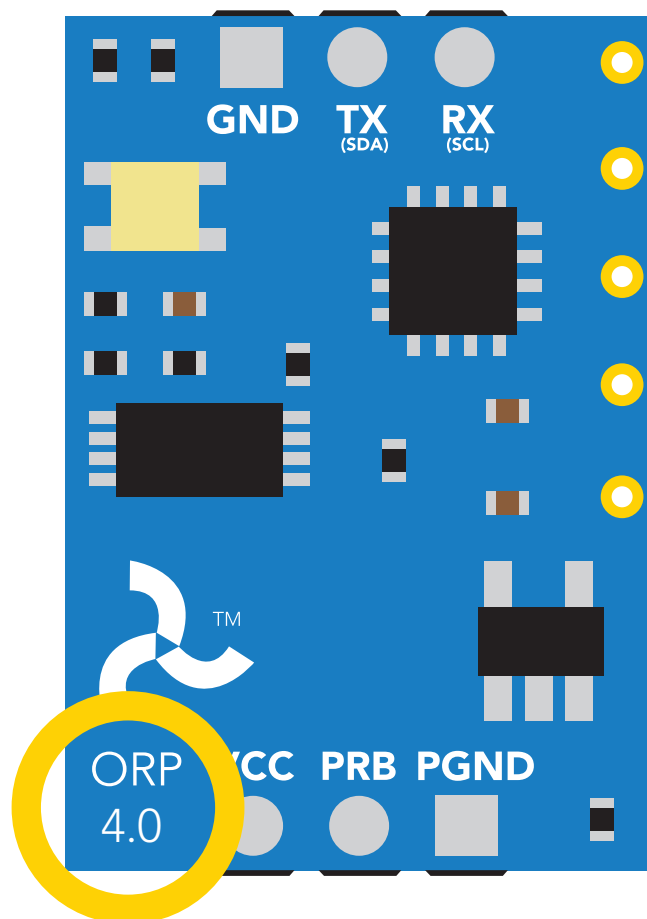

Legacy ORP circuit




Viewing incorrect datasheet

[Click here to view legacy datasheet](#)

Operating principle

ORP stands for **oxidation/reduction potential**. Oxidation is the loss of electrons and reduction is the gain of electrons. The output of the probe is represented in millivolts and can be positive or negative.

Just like a pH probe measures hydrogen ion activity in a liquid; an ORP probe measures electron activity in a liquid. The ORP readings represents how strongly electrons are transferred to or from substances in a liquid. Keeping in mind that the readings do not indicate the amount of electrons available for transfer.

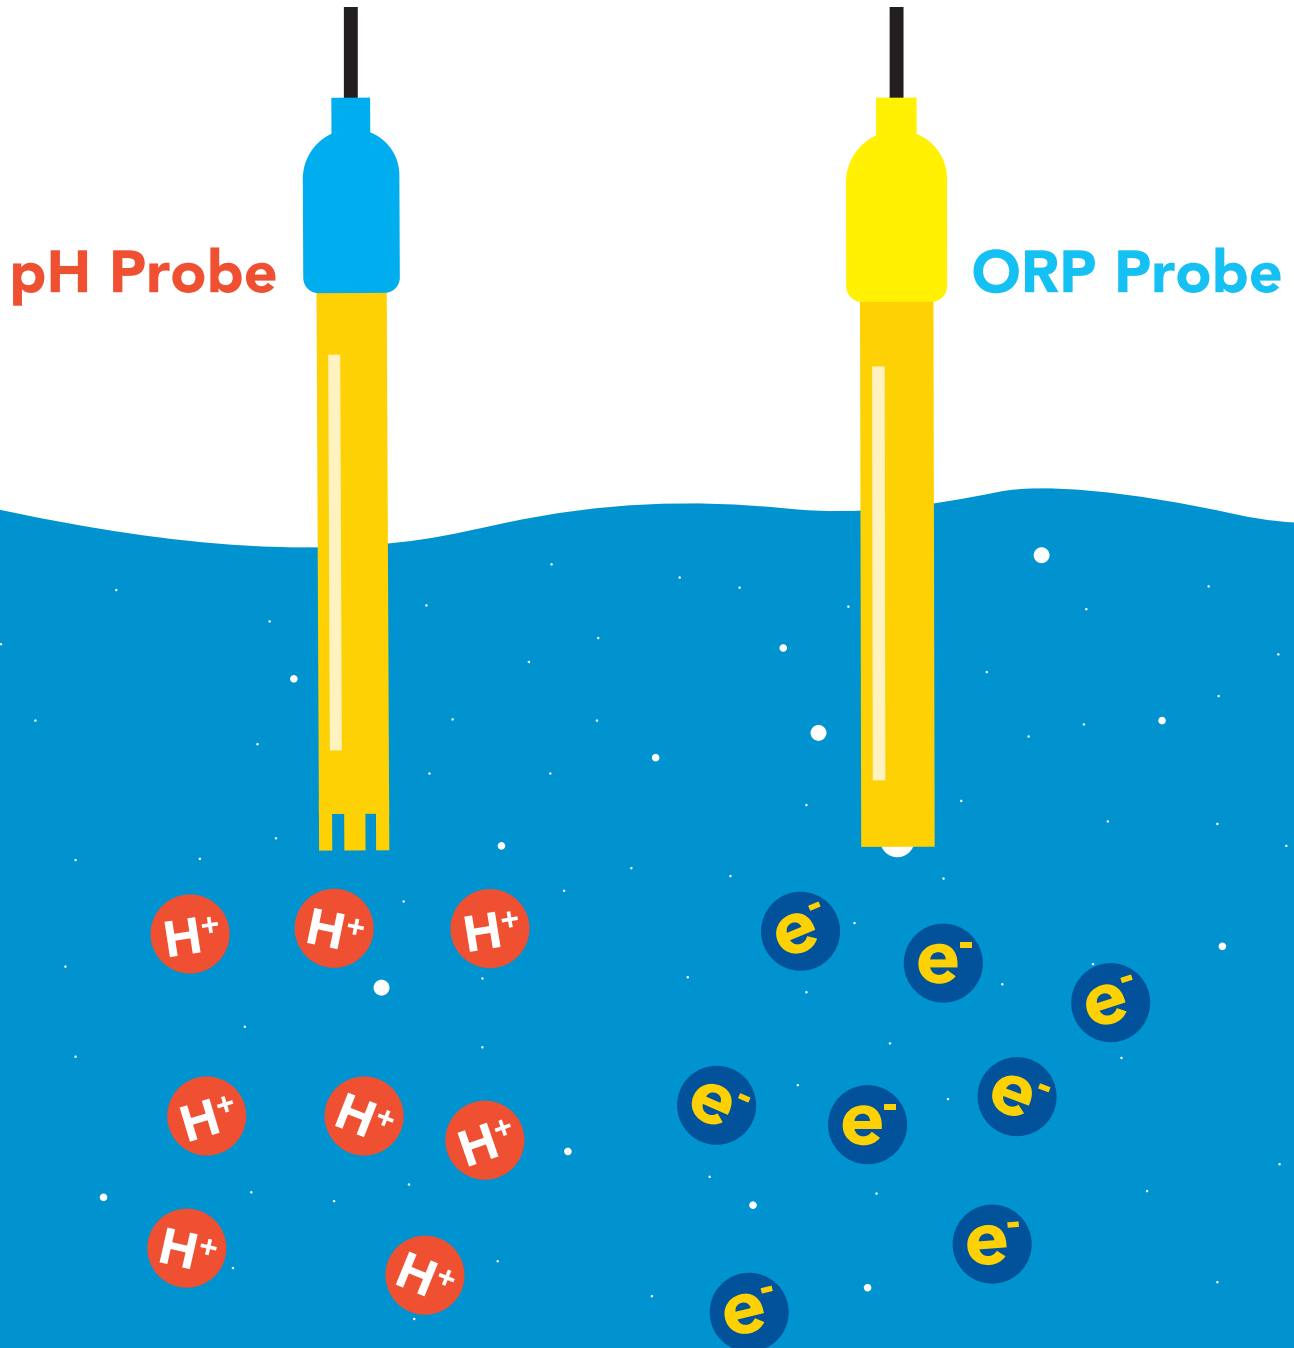


When reading the ORP of a liquid that has very few electrons available for transfer ORP readings can appear to be inconsistent.

The water is unreactive and has only trace amounts of electron movement. *These readings are equivalent to the readings you see with an unconnected multimeter.*

-234.6

Reading A

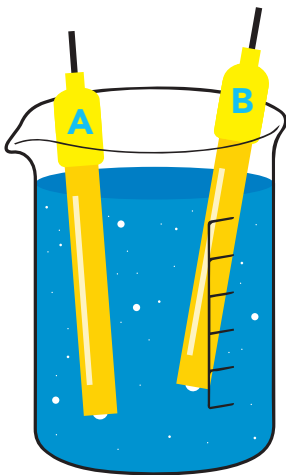


24.2

Reading B

Tap water

606.9

Reading A

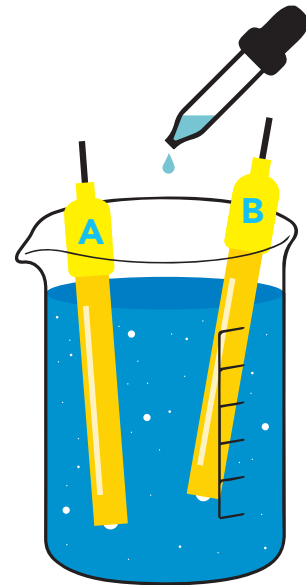


605.3

Reading B

Tap water

Add just a drop of bleach
(which is an oxidizing agent)

An ORP probe has a platinum tip that is connected to a silver wire, surrounded by silver chloride. That silver wire is then connected to a KCL reference solution. Because platinum is an unreactive metal it can “silently observe” the electron activity of the liquid without becoming apart of whatever reaction is occurring in the liquid.

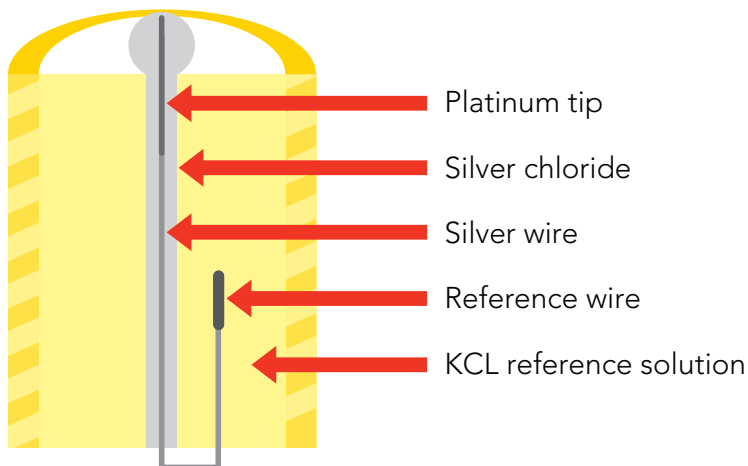

Calibration theory


The most important part of calibration is watching the readings during the calibration process. It's easiest to calibrate the device in its default state (UART mode, continuous readings). Switching the device to I²C mode after calibration **will not** affect the stored calibration. If the device must be calibrated in I²C mode be sure to request readings continuously so you can see the output from the probe.

Calibration should be done at least once per year.

If the ORP that's being read is continuously on the extremes of the scale (around -900mV or +900mV) calibration may have to be done more often. The exact frequency of calibration will have to be determined by your engineering team.

The Atlas Scientific EZO™ class ORP circuit has a flexible calibration protocol, allowing single point calibration to any off the shelf calibration solution.

Single point calibration

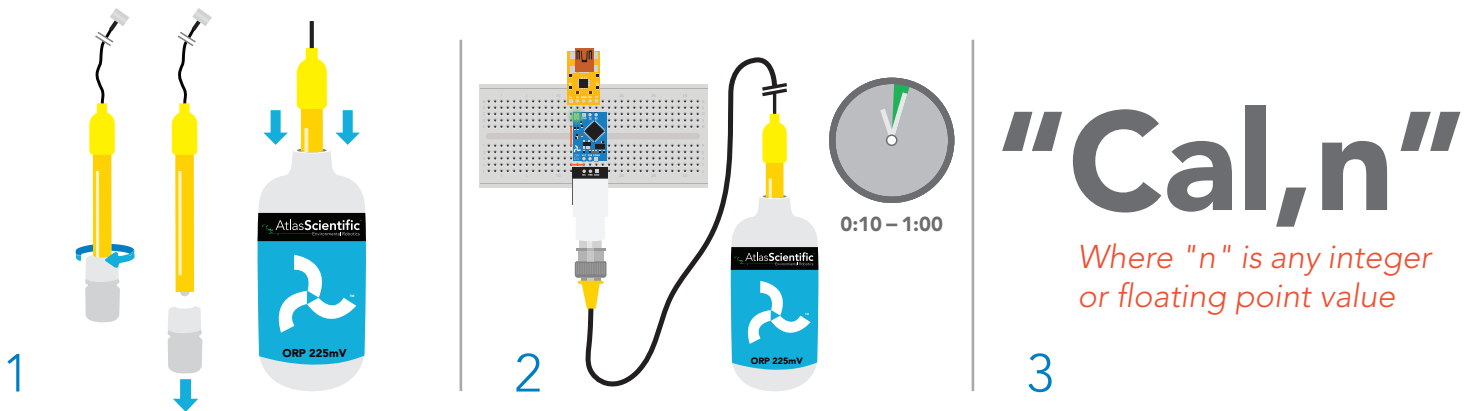


1. Remove soaker bottle and place probe in ORP calibration solution.
2. Let the probe sit in calibration solution until readings stabilize (10 – 60 seconds).
3. Calibrate to the value of the calibration solution using the command "Cal,n".

(If you are using the Atlas Scientific ORP calibration solution, calibrate to 225mV; "Cal,225").


Power and data isolation

The Atlas Scientific EZO™ ORP circuit is a very sensitive device. This sensitivity is what gives the ORP circuit its accuracy. This also means that the ORP circuit is capable of reading micro-voltages that are bleeding into the water from unnatural sources such as pumps, solenoid valves or other probes/sensors.


When electrical noise is interfering with the ORP readings it is common to see rapidly fluctuating readings or readings that are consistently off. To verify that electrical noise is causing inaccurate readings, place the ORP probe in a cup of water by itself. The readings should stabilize quickly, confirming that electrical noise was the issue.

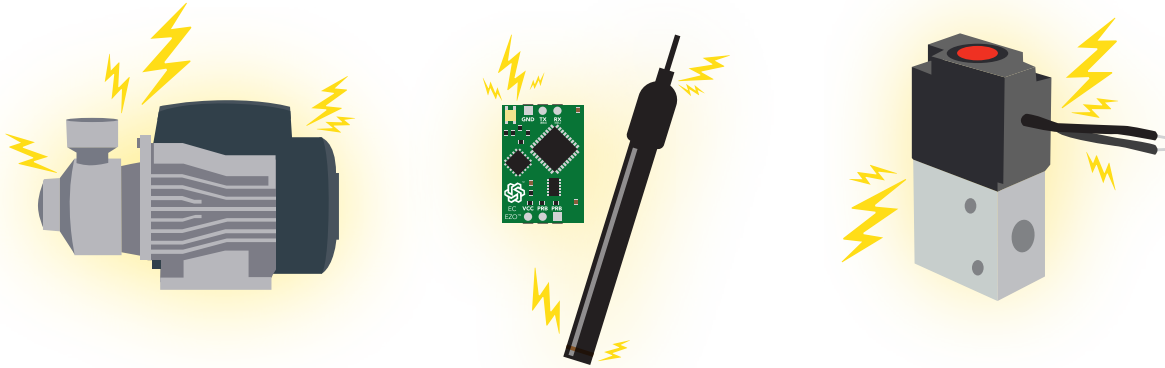

When reading ORP and Conductivity or Dissolved Oxygen together, it is **strongly recommended** that the EZO™ ORP circuit is electrically isolated from the EZO™ Conductivity or Dissolved Oxygen circuit.

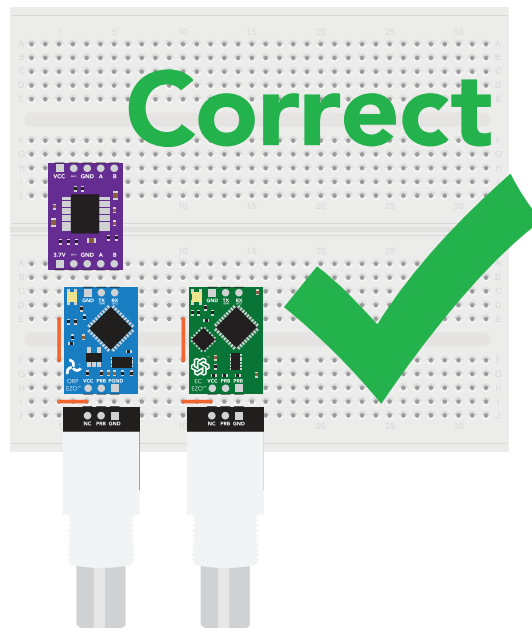

Basic EZO™
Inline Voltage Isolator

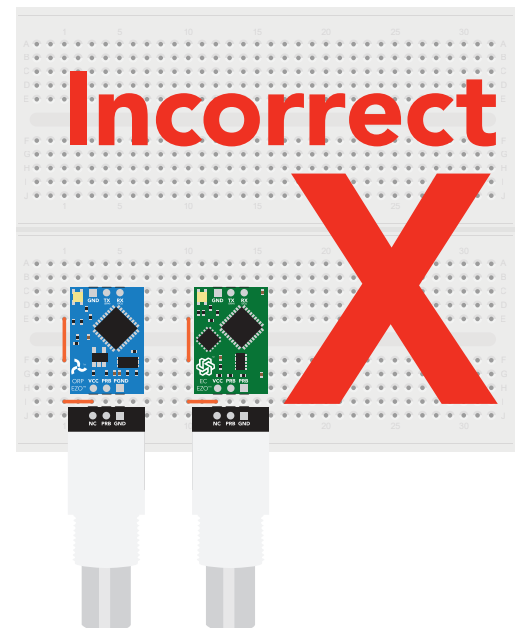


Without isolation, Conductivity and Dissolved Oxygen readings will effect ORP accuracy.

This schematic shows exactly how we isolate data and power using the [ADM3260](#) and a few passive components. The ADM3260 can output isolated power up to 150 mW and incorporates two bidirectional data channels.


This technology works by using tiny transformers to induce the voltage across an air gap. PCB layout requires special attention for EMI/EMC and RF Control, having proper ground planes and keeping the capacitors as close to the chip as possible are crucial for proper performance. The two data channels have a 4.7k Ω pull up resistor on both the isolated and non-isolated lines (R1, R2, R3, and R4) The output voltage is set using a voltage divider (R5, R6, and R7) this produces a voltage of 3.7V regardless of your input voltage.

Isolated ground is different from non-isolated ground, these two lines should not be connected together.

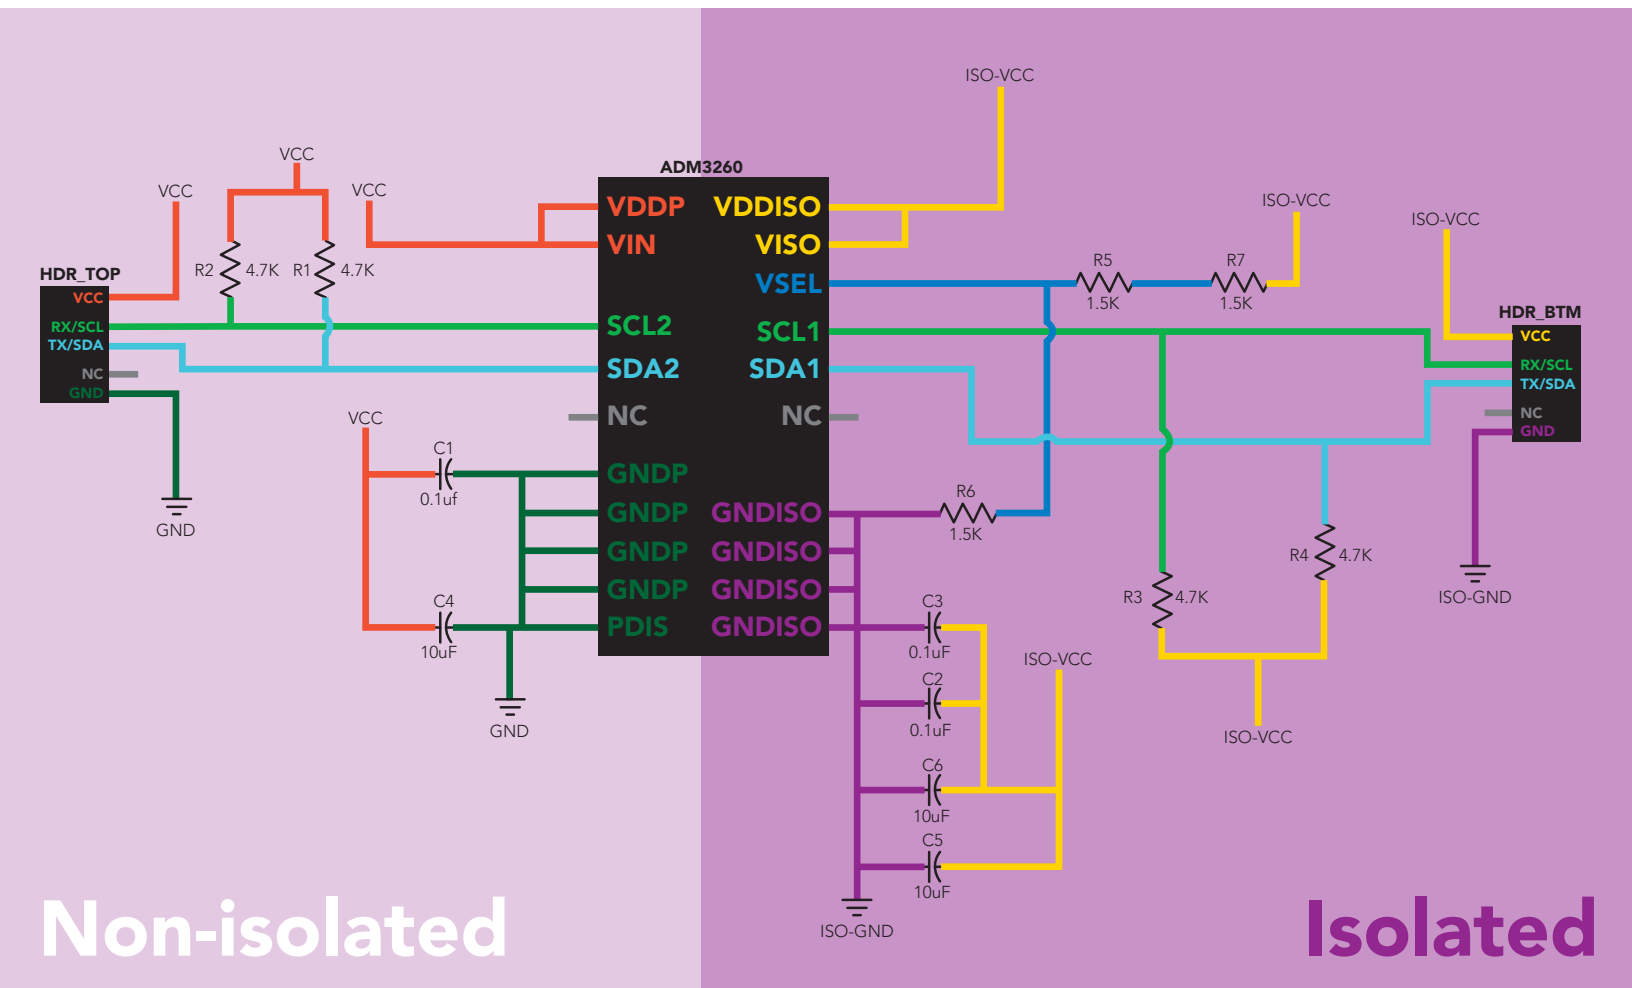


✓ Correct wiring


Bread board

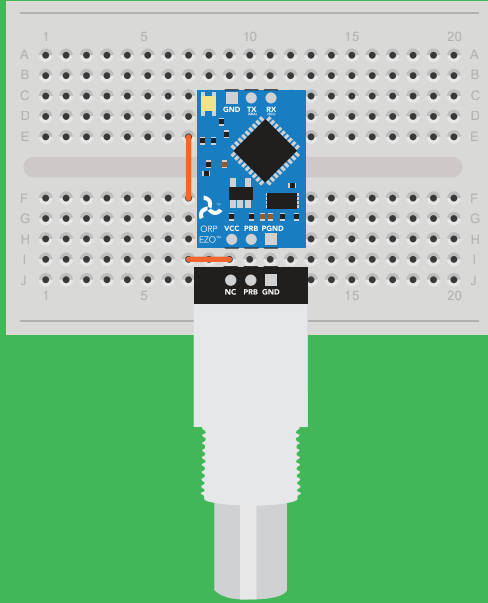


Bread board via USB

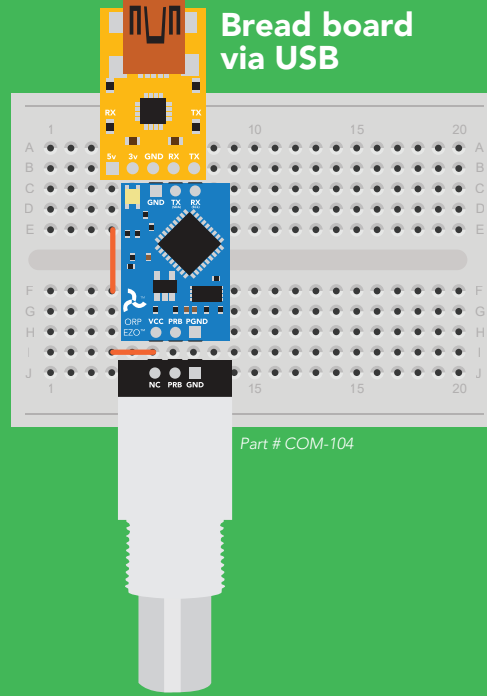

Carrier board

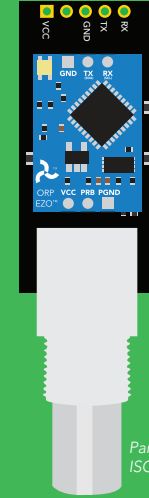


USB carrier board

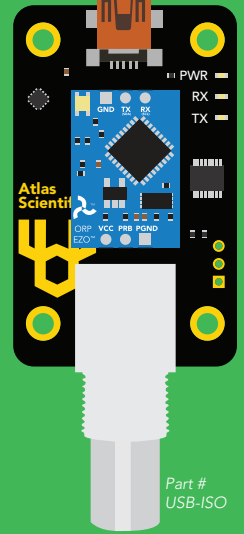


X Incorrect wiring


Extended leads

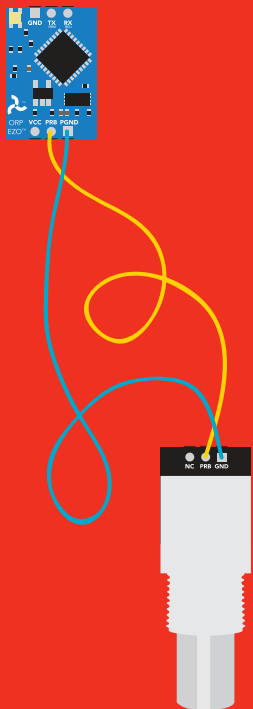

Sloppy setup

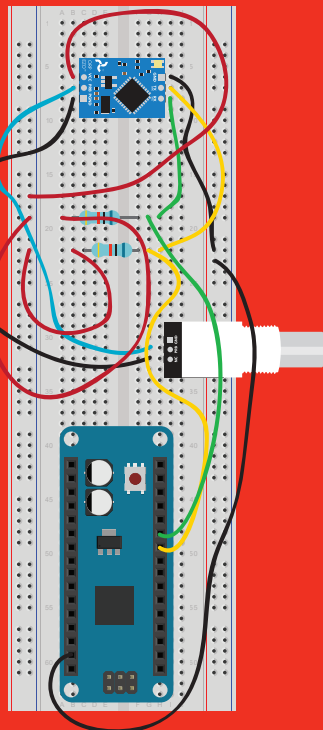


Perfboards or Protoboards

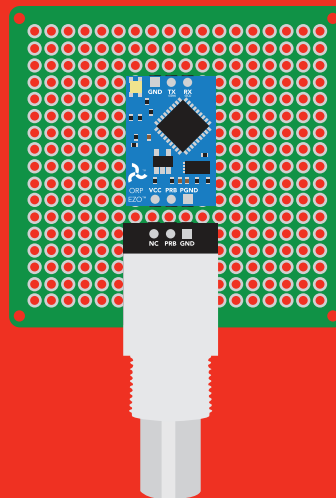



NEVER
use Perfboards
or Protoboards

*Embedded into your device

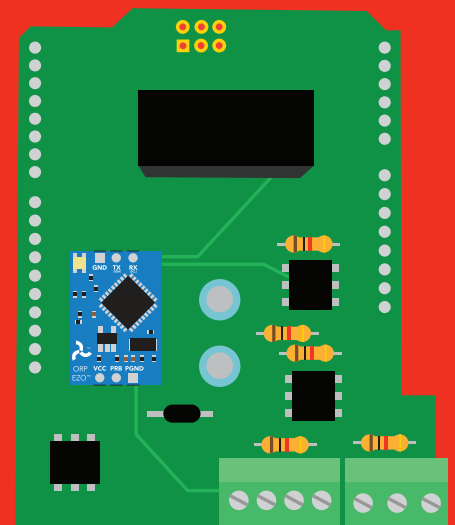


***Only after you are familiar
with EZO™ circuits operation**

NEVER EXTEND THE CABLE
WITH CHEAP JUMPER WIRES!

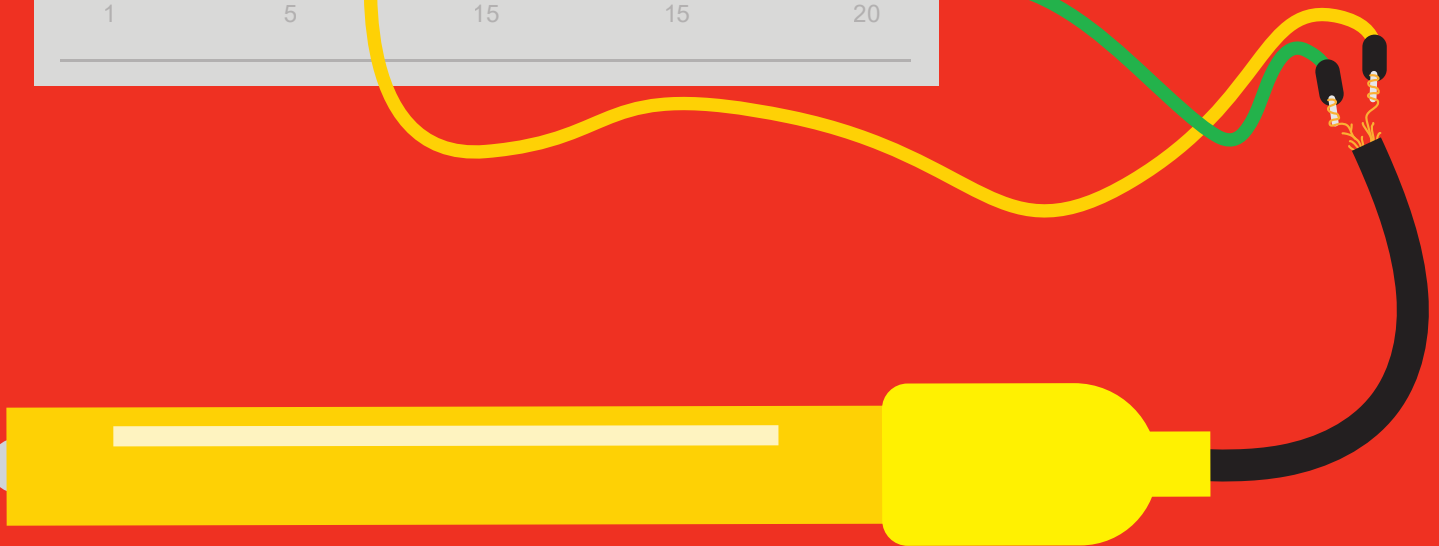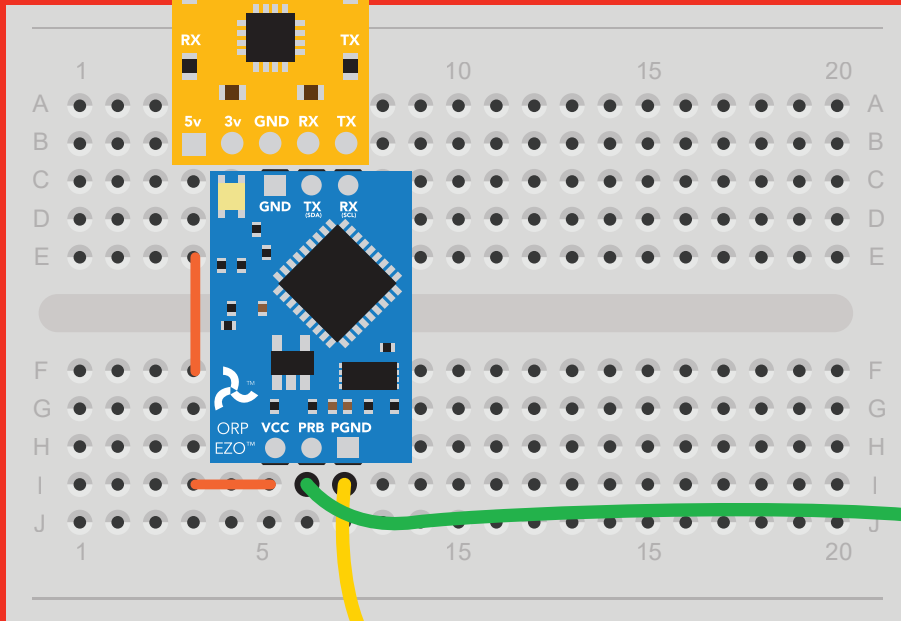

**DO NOT CUT THE PROBE CABLE
WITHOUT REFERRING TO **THIS DOCUMENT!****

**DO NOT MAKE YOUR OWN
UNSHIELDED CABLES!**

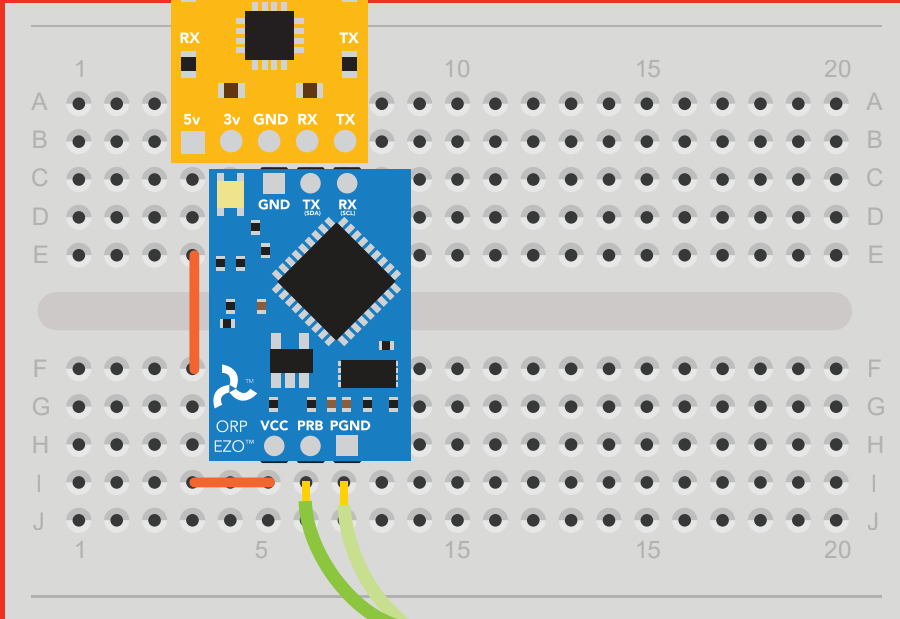

**ONLY USE SHIELDED CABLES.
REFER TO **THIS DOCUMENT!****

✓ Available data protocols

UART

Default

I²C

✗ Unavailable data protocols

SPI

Analog

RS-485

Mod Bus

4–20mA

UART mode

Settings that are retained if power is cut

- Baud rate
- Calibration
- Continuous mode
- Device name
- Enable/disable response codes
- Hardware switch to I²C mode
- LED control
- Protocol lock
- Software switch to I²C mode

Settings that are **NOT** retained if power is cut

- Find
- Sleep mode

UART mode

8 data bits
1 stop bit

no parity
no flow control

Baud 300
1,200
2,400
9,600 default
19,200
38,400
57,600
115,200

RX
Data in



TX
Data out




Vcc 3.3V – 5.5V

0V



VCC

0V

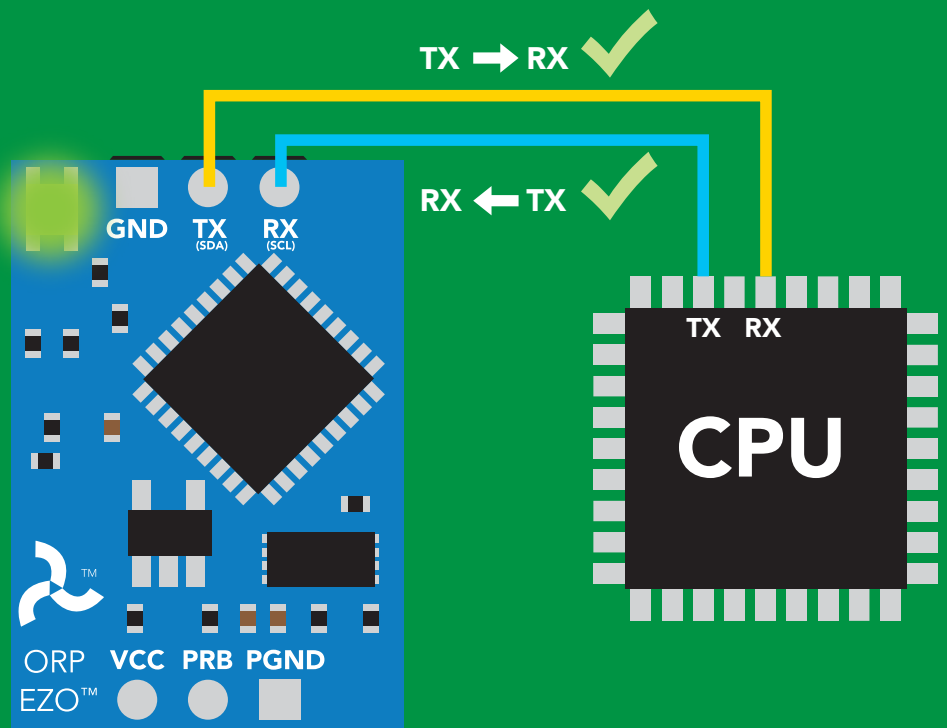


Data format

Reading	ORP	Data type	floating point
Units	mV	Decimal places	1
Encoding	ASCII	Smallest string	2 characters
Format	string	Largest string	40 characters
Terminator	carriage return		

Default state

Mode	UART
Baud	9,600
Readings	continuous
Speed	1 reading per second
LED	on

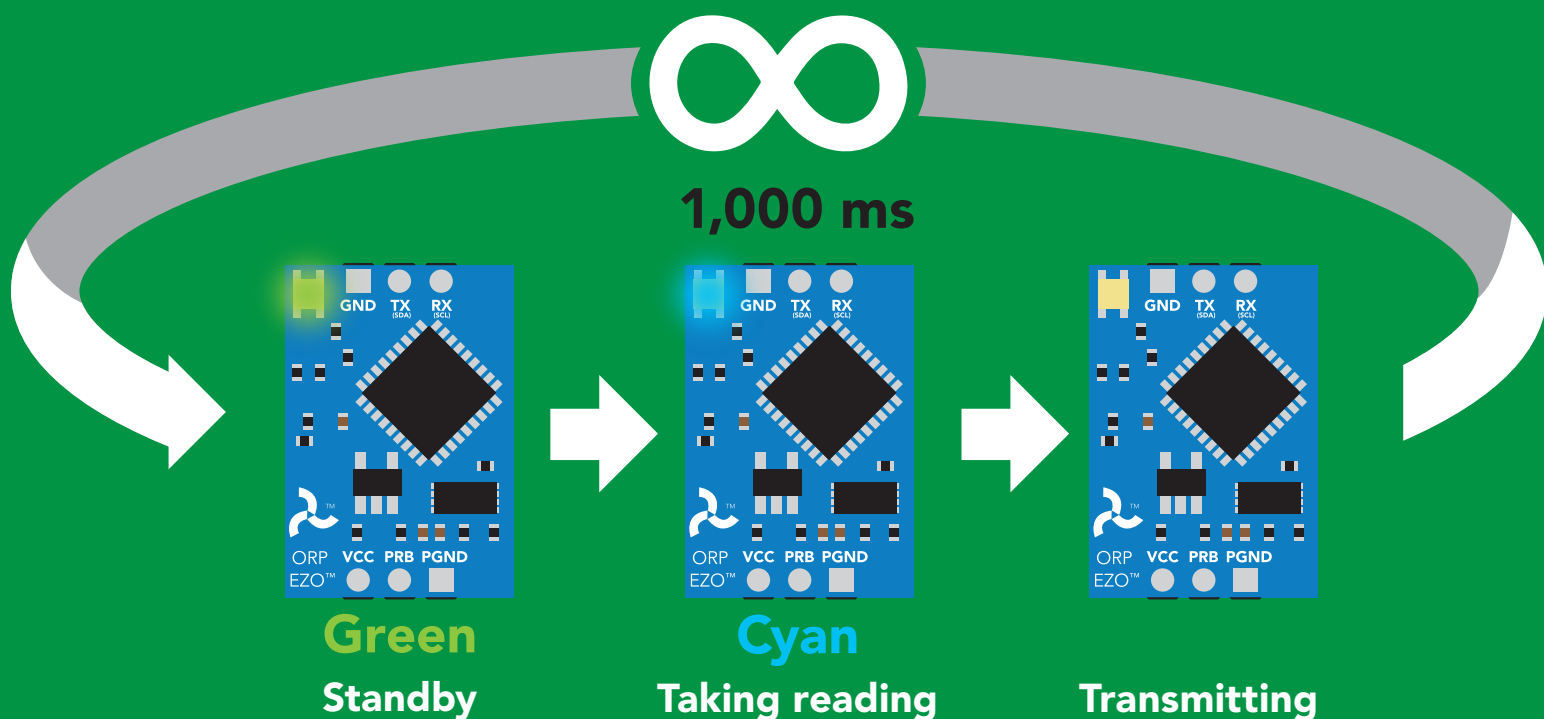

Receiving data from device


2 parts

ASCII data string

Command

Carriage return <cr>

Terminator

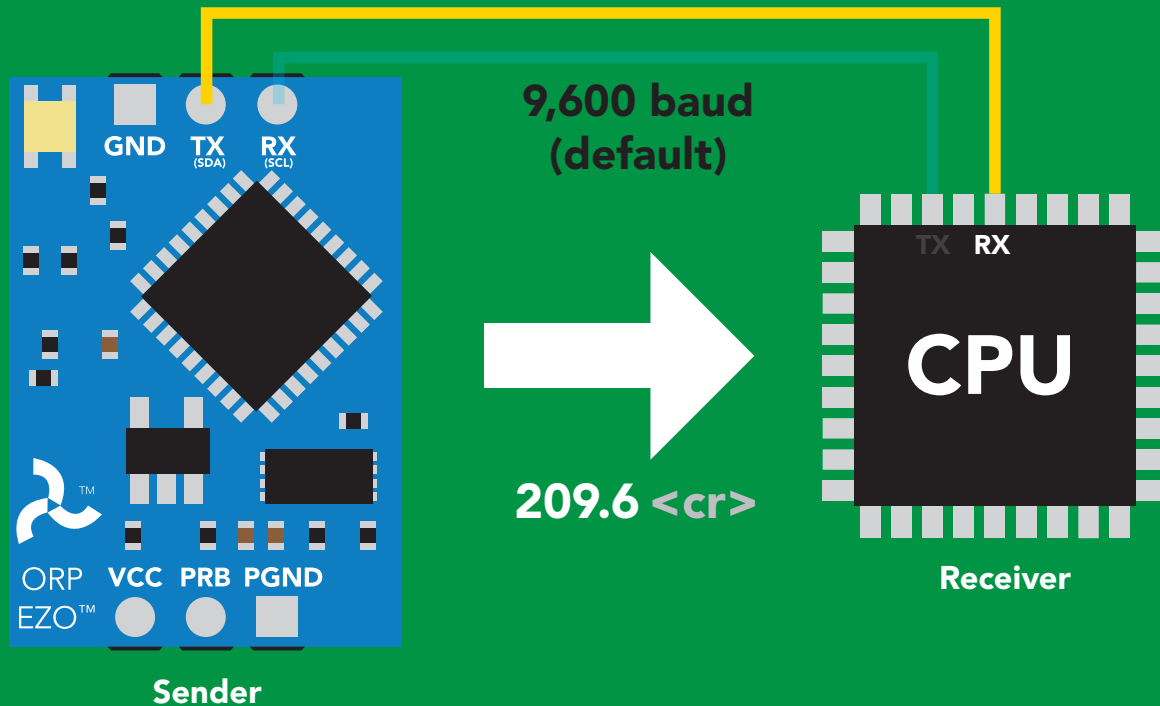

Advanced

ASCII: 2 0 9 . 6 <cr>

Hex: 32 30 39 2E 36 0D

Dec: 50 48 57 46 54 13

Sending commands to device


2 parts

Command (not case sensitive)

ASCII data string

Carriage return <cr>

Terminator

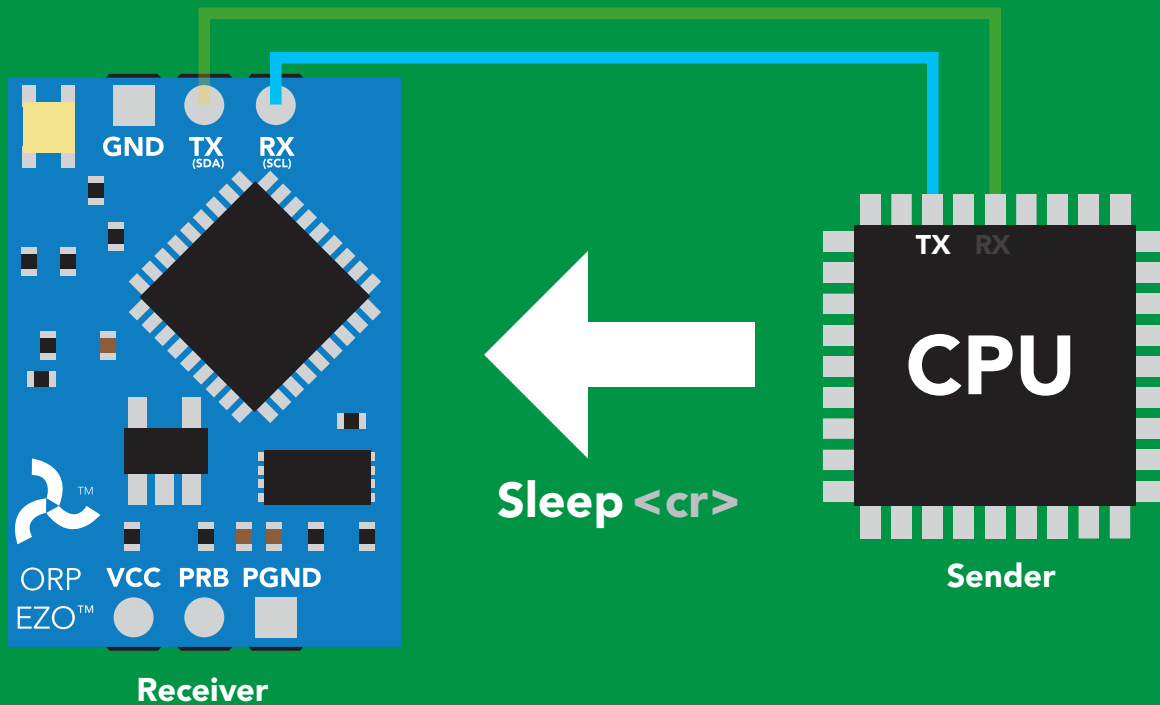


Advanced

ASCII: **S** **I** **e** **e** **p** **<cr>**


Hex: **53** **6C** **65** **65** **70** **0D**

Dec: **83** **108** **101** **101** **112** **13**


LED color definition

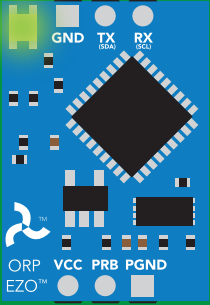


Green
UART standby

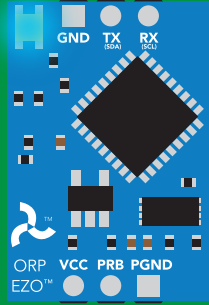


Cyan
Taking reading

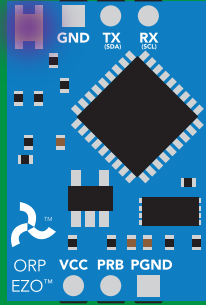

Purple
Changing
baud rate

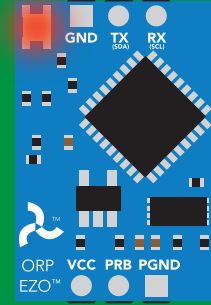

Red
Command
not understood

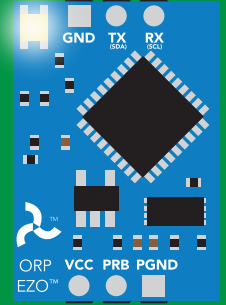

White
Find

5V

LED ON
+2.2 mA

3.3V

+0.6 mA

UART mode

command quick reference

All commands are ASCII strings or single ASCII characters.

Command	Function		Default state
Baud	change baud rate	pg. 33	9,600
C	enable/disable continuous reading	pg. 24	enabled
Cal	performs calibration	pg. 26	n/a
Export/import	export/import calibration	pg. 27	n/a
Factory	enable factory reset	pg. 35	n/a
Find	finds device with blinking white LED	pg. 23	n/a
i	device information	pg. 29	n/a
I2C	change to I ² C mode	pg. 36	not set
L	enable/disable LED	pg. 22	enabled
Name	set/show name of device	pg. 28	not set
Plock	enable/disable protocol lock	pg. 34	disabled
R	returns a single reading	pg. 25	n/a
Sleep	enter sleep mode/low power	pg. 32	n/a
Status	retrieve status information	pg. 31	n/a
*OK	enable/disable response codes	pg. 30	enable

LED control

Command syntax

L,1 <cr> LED on **default**

L,0 <cr> LED off

L,? <cr> LED state on/off?

Example

Response

L,1 <cr>


*OK <cr>

L,0 <cr>


*OK <cr>

L,? <cr>

?L,1 <cr> or ?L,0 <cr>
*OK <cr>

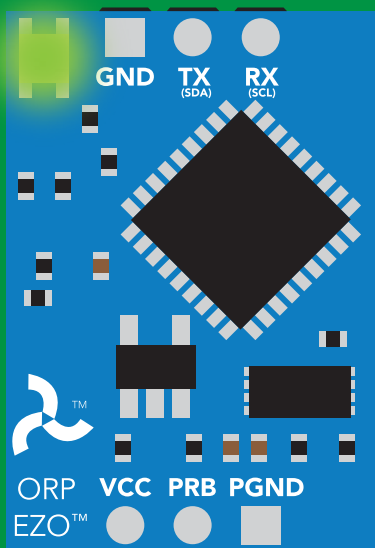

L,1

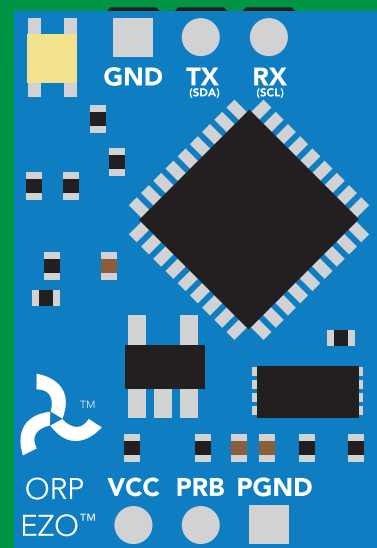

L,0

Find

Command syntax

This command will disable continuous mode
Send any character or command to terminate find.


Find <cr> LED rapidly blinks white, used to help find device

Example

Find <cr>

Response

***OK** <cr>

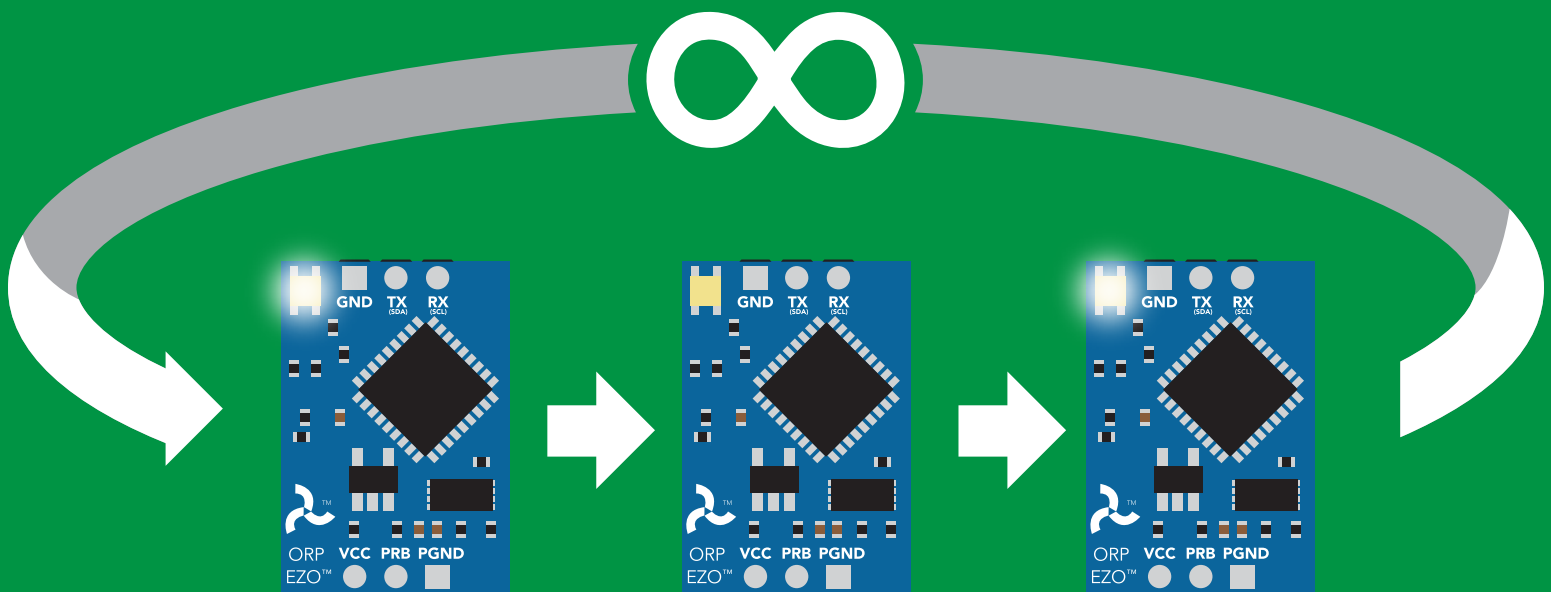

Continuous reading mode

Command syntax

- C,1 <cr>** enable continuous readings once per second **default**
- C,n <cr>** continuous readings every n seconds (n = 2 to 99 sec)
- C,0 <cr>** disable continuous readings
- C,? <cr>** continuous reading mode on/off?

Example

Response

C,1 <cr>

***OK <cr>**
ORP (1 sec) <cr>
ORP (2 sec) <cr>
ORP (n sec) <cr>

C,30 <cr>

***OK <cr>**
ORP (30 sec) <cr>
ORP (60 sec) <cr>
ORP (90 sec) <cr>

C,0 <cr>

***OK <cr>**

C,? <cr>

?C,1 <cr> or ?C,0 <cr> or ?C,30 <cr>
***OK <cr>**

Single reading mode

Command syntax


R <cr> takes single reading

Example


R <cr>

Response


209.6 <cr>
*OK <cr>

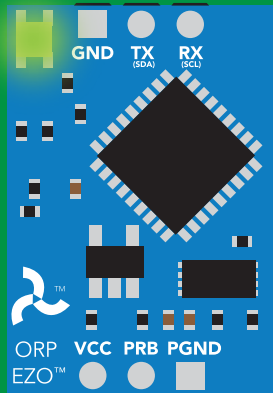

Green
Standby

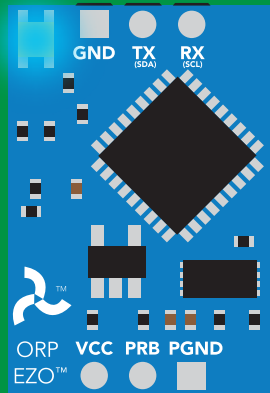

Cyan
Taking reading

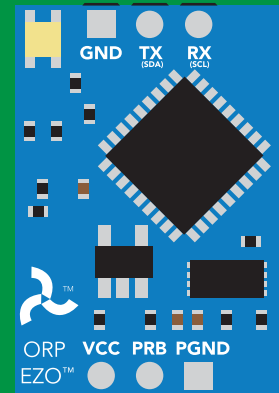

Transmitting



800 ms

Calibration

Command syntax

The EZO™ ORP circuit can be calibrated to any known ORP value

Cal,n <cr> calibrates the ORP circuit to a set value

Cal,clear <cr> delete calibration data

Cal,? <cr> device calibrated?

Example

Response

Cal,225 <cr>


***OK** <cr>

Cal,clear <cr>

***OK** <cr>

Cal,? <cr>

?Cal,0 <cr> **or** **?Cal,1** <cr>
***OK** <cr>

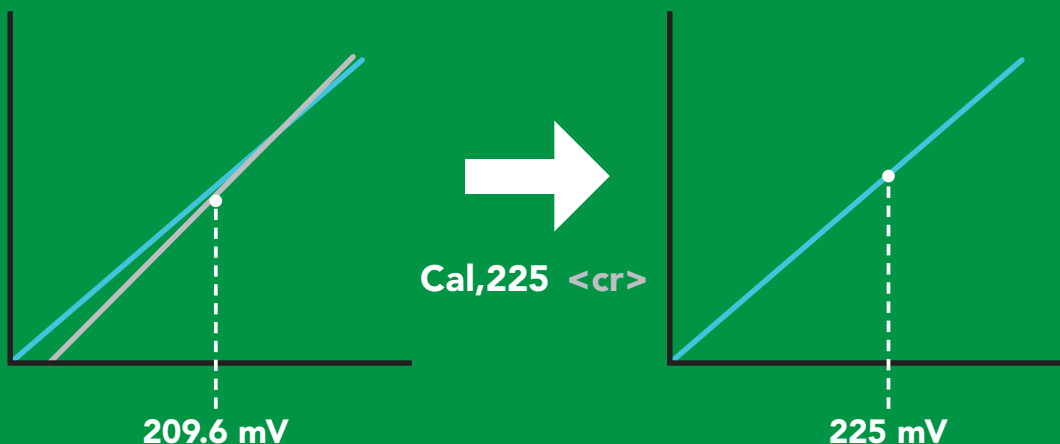

Export/import calibration

Command syntax

Export: Use this command to save calibration settings
Import: Use this command to load calibration settings to one or more devices.

Export <cr> export calibration string from calibrated device
Import <cr> import calibration string to new device
Export,? <cr> calibration string info

Example

Response

Export,? <cr>

10,120 <cr>

Response breakdown

10, 120

↑ ↑
of strings to export # of bytes to export

Export strings can be up to 12 characters long,
and is always followed by <cr>

Export <cr>

59 6F 75 20 61 72 <cr> **(1 of 10)**

Export <cr>

65 20 61 20 63 6F <cr> **(2 of 10)**

(7 more)

⋮

Export <cr>

6F 6C 20 67 75 79 <cr> **(10 of 10)**

Export <cr>

***DONE**

Disabling *OK simplifies this process

Import, n
(FIFO)

Import, 59 6F 75 20 61 72 <cr> **(1 of 10)**

Naming device

Command syntax

Name,n <cr> set name

Name,? <cr> show name

n =

1 2 3 4 5 6 7 8 9 10 11 12 13 14 15 16

Up to 16 ASCII characters

Example

Response


Name,zzt <cr>

*OK <cr>

Name,? <cr>


?Name,zzt <cr>
*OK <cr>

Name,zzt

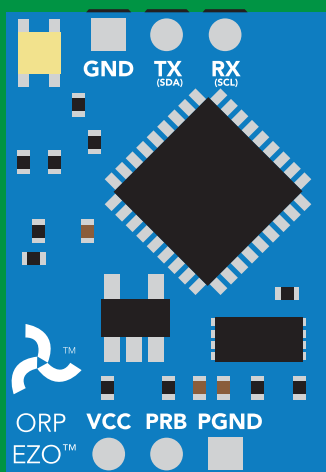

*OK <cr>

Name,?

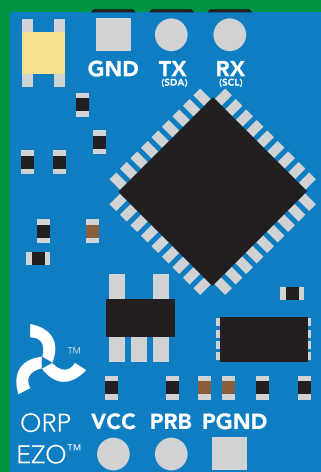

Name,zzt <cr>
*OK <cr>

Device information

Command syntax

```
i <cr> device information
```

Example

```
i <cr>
```

Response

```
?i,ORP,1.97 <cr>  
*OK <cr>
```

Response breakdown

?i,	ORP,	1.97
	↑	↑
	Device	Firmware

Response codes

Command syntax

- *OK,1** <cr> enable response **default**
- *OK,0** <cr> disable response
- *OK,?** <cr> response on/off?

Example

Response

R <cr>

209.6 <cr>
***OK** <cr>

***OK,0** <cr>

no response, ***OK** disabled

R <cr>

209.6 <cr> ***OK** disabled

***OK,?** <cr>

?*OK,1 <cr> or **?*OK,0** <cr>

Other response codes

- *ER** unknown command
- *OV** over volt ($VCC \geq 5.5V$)
- *UV** under volt ($VCC \leq 3.1V$)
- *RS** reset
- *RE** boot up complete, ready
- *SL** entering sleep mode
- *WA** wake up

These response codes
cannot be disabled

Reading device status

Command syntax

Status <cr> voltage at Vcc pin and reason for last restart

Example

Status <cr>

Response

?Status,P,5.038 <cr>
*OK <cr>

Response breakdown

?Status,	P,	5.038
	↑	↑
	Reason for restart	Voltage at Vcc

Restart codes

P	powered off
S	software reset
B	brown out
W	watchdog
U	unknown

Sleep mode/low power

Command syntax

Send any character or command to awaken device.

Sleep <cr> enter sleep mode/low power

Example

Response

Sleep <cr>

***SL**

Any command

***WA** <cr> wakes up device

5V

STANDBY

16 mA


SLEEP

1.16 mA


3.3V

13.9 mA


0.995 mA

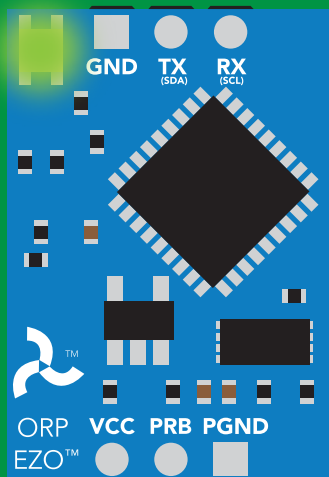

**Standby
16 mA**



Sleep <cr>

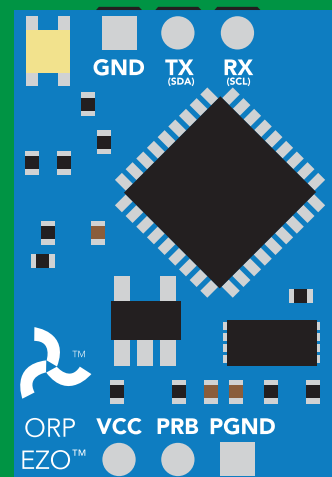

**Sleep
1.16 mA**

Change baud rate

Command syntax

Baud,n <cr> change baud rate

Example

Baud,38400 <cr>

Response

*OK <cr>


Baud,? <cr>

?Baud,38400 <cr>

*OK <cr>


n =

- 300
- 1200
- 2400
- 9600 default**
- 19200
- 38400
- 57600
- 115200

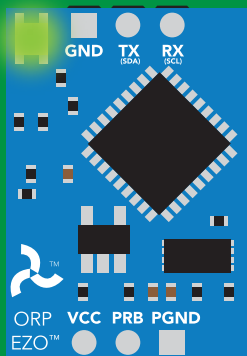


Standby

Baud,38400 <cr>

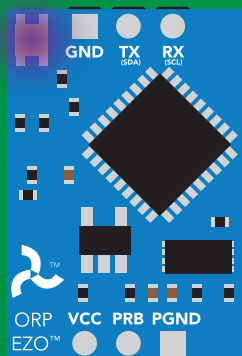


Changing
baud rate

*OK <cr>



(reboot)

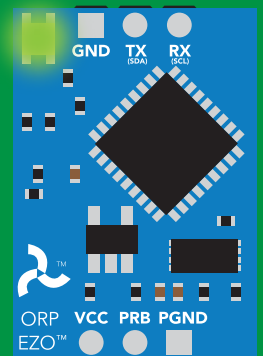

Standby

Protocol lock

Command syntax

Locks device to UART mode.

Plock,1 <cr> enable Plock

Plock,0 <cr> disable Plock **default**

Plock,? <cr> Plock on/off?

Example

Plock,1 <cr>

*OK <cr>


Plock,0 <cr>

*OK <cr>

Plock,? <cr>


?Plock,1 <cr> or ?Plock,0 <cr>

Plock,1

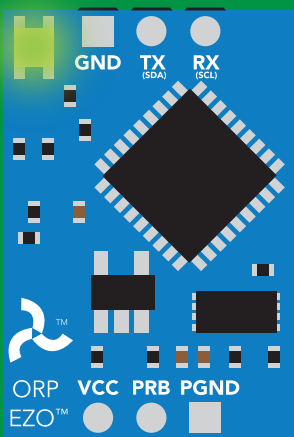


*OK <cr>

I2C,100

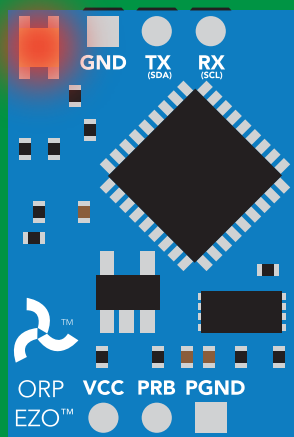

cannot change to I²C
*ER <cr>

Short

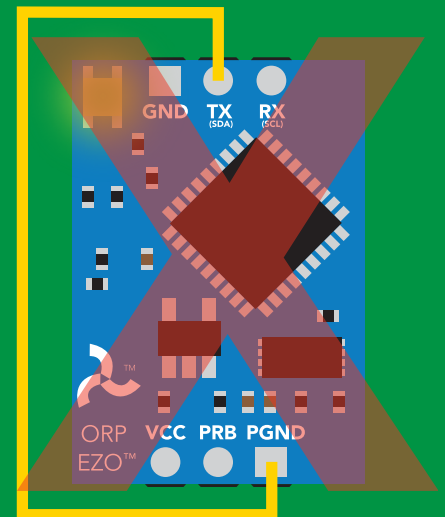

cannot change to I²C

Factory reset

Command syntax

Clears calibration
LED on
"*OK" enabled

Factory <cr> enable factory reset


Example

Response


Factory <cr>

*OK <cr>

Factory <cr>

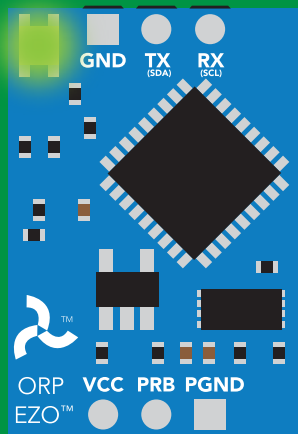

(reboot)

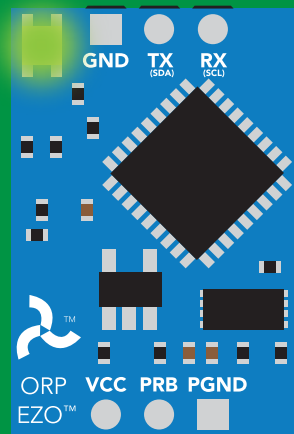

*OK <cr>

*RS <cr>

*RE <cr>

Baud rate will not change

Change to I²C mode

Command syntax

Default I²C address 98 (0x62)

I2C,n <cr> sets I²C address and reboots into I²C mode

n = any number 1 – 127

Example

I2C,100 <cr>

Response

*OK (reboot in I²C mode)


Wrong example

I2C,139 <cr> n ≠ 127

Response


*ER <cr>

I2C,100

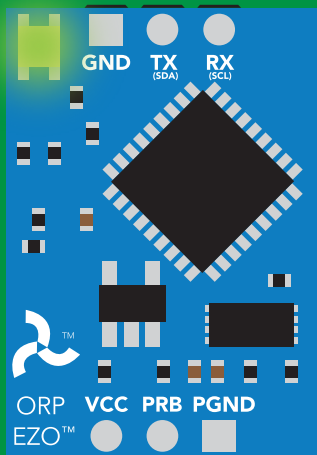


Green

*OK <cr>



(reboot)

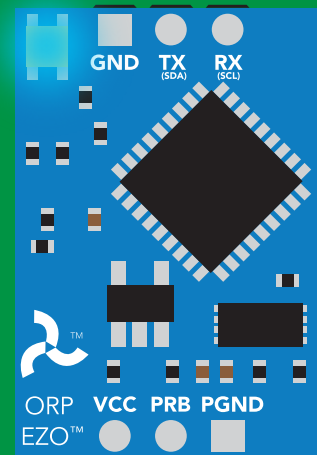

Blue


now in I²C mode

Manual switching to I²C


- Make sure Plock is set to 0
- Disconnect ground (power off)
- Disconnect TX and RX
- Connect TX to PGND
- Confirm RX is disconnected
- Connect ground (power on)
- Wait for LED to change from **Green** to **Blue**
- Disconnect ground (power off)
- Reconnect all data and power

Manually switching to I²C will set the I²C address to 98 (0x62)

Example

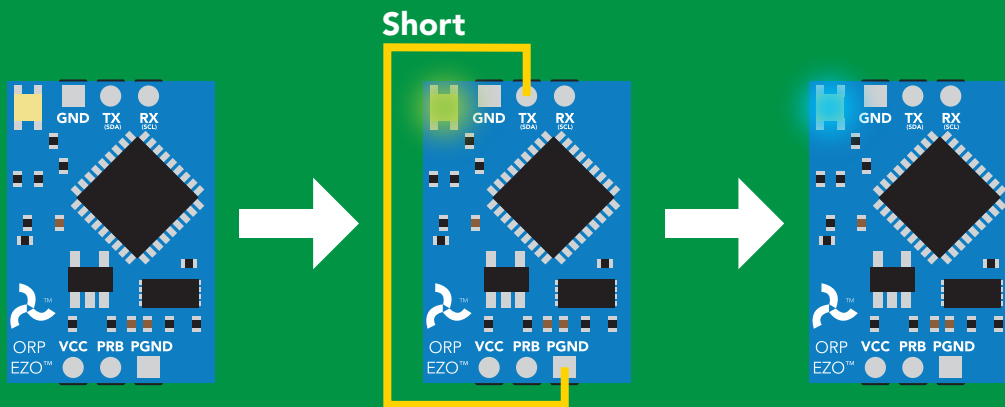

Wrong Example

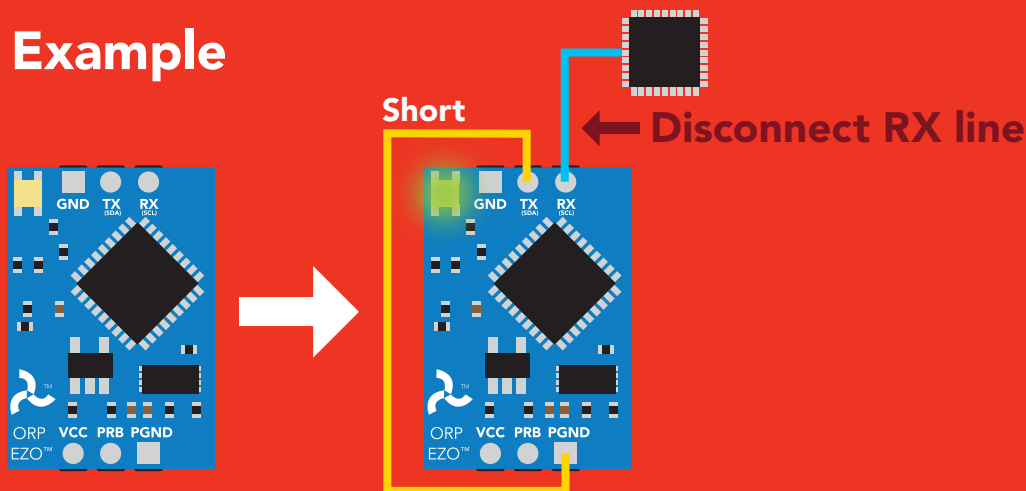

I²C mode

The I²C protocol is **considerably more complex** than the UART (RS-232) protocol. Atlas Scientific assumes the embedded systems engineer understands this protocol.

To set your EZO™ device into I²C mode [click here](#)

Settings that are retained if power is cut

- Calibration
- Change I²C address
- Hardware switch to UART mode
- LED control
- Protocol lock
- Software switch to UART mode

Settings that are **NOT** retained if power is cut

- Find
- Sleep mode

I²C mode

I²C address (0x01 – 0x7F)
98 (0x62) default


V_{cc} 3.3V – 5.5V

Clock speed 100 – 400 kHz

SDA 

SCL 


 VCC
0V 0V

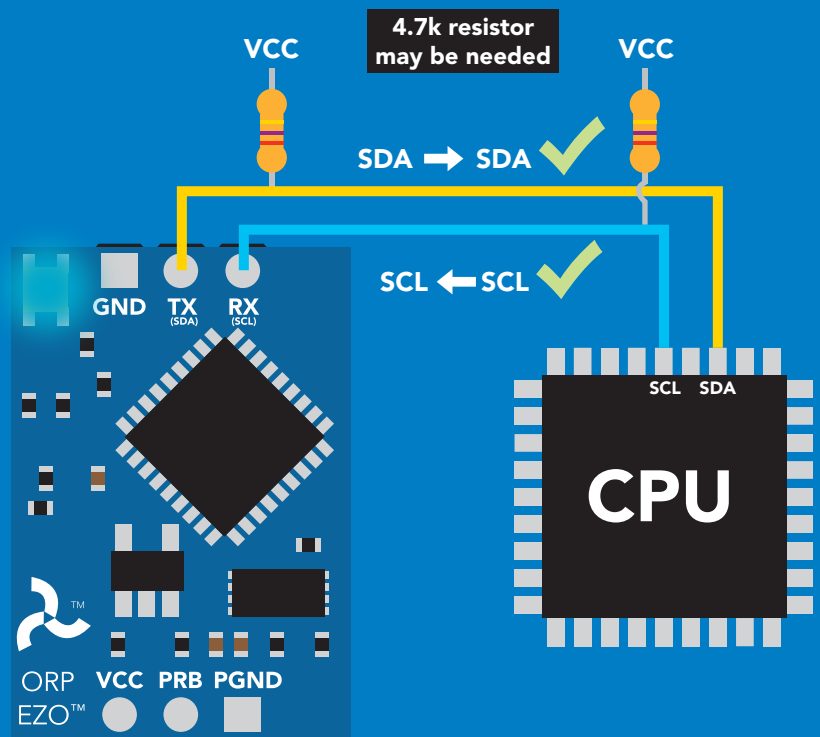


Data format

Reading	ORP	Data type	floating point
Units	mV	Decimal places	1
Encoding	ASCII	Smallest string	2 characters
Format	string	Largest string	399 characters


Sending commands to device

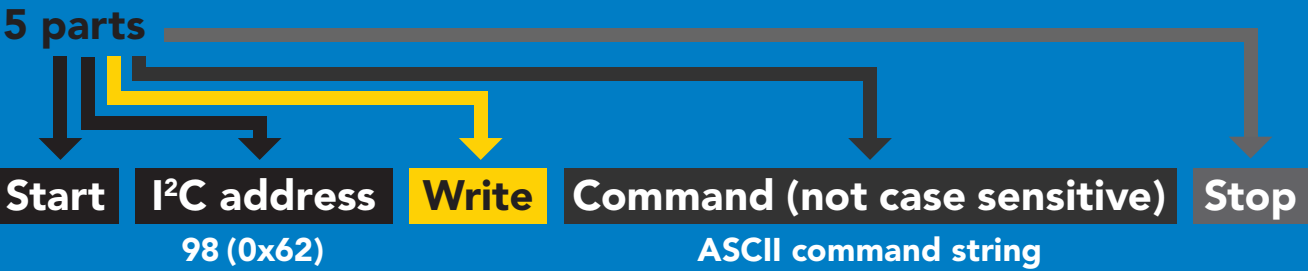



Example

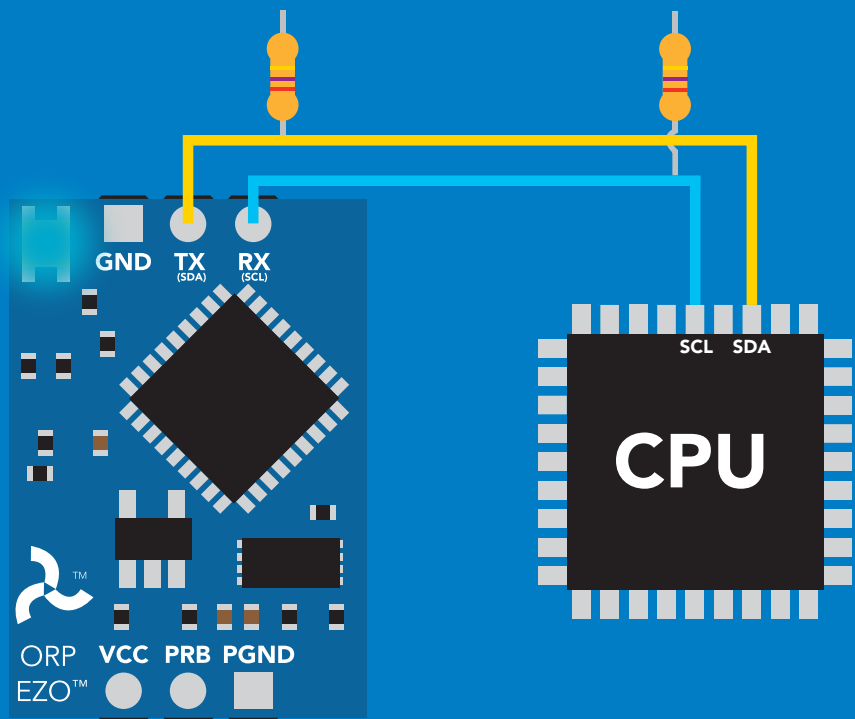


Advanced

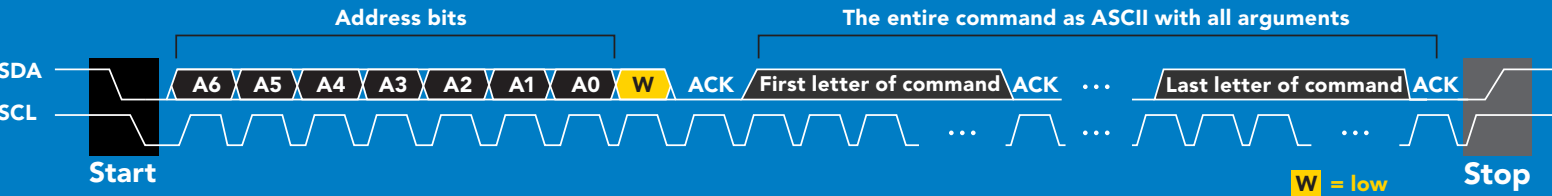

Requesting data from device

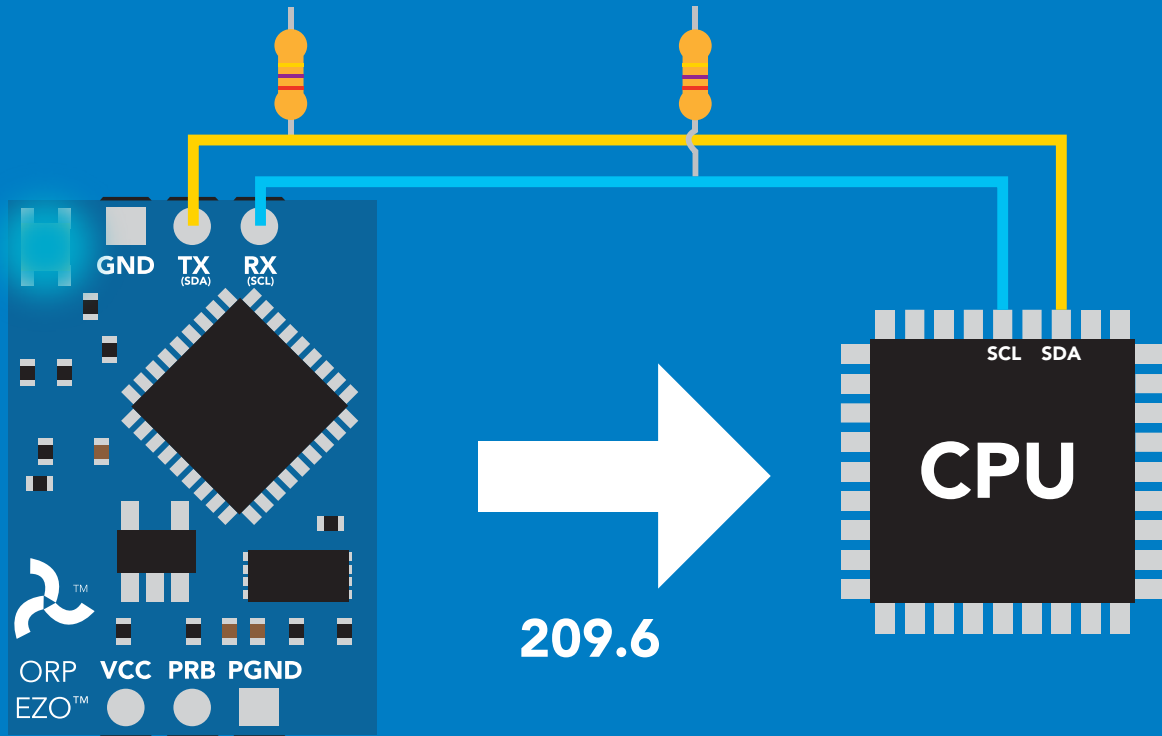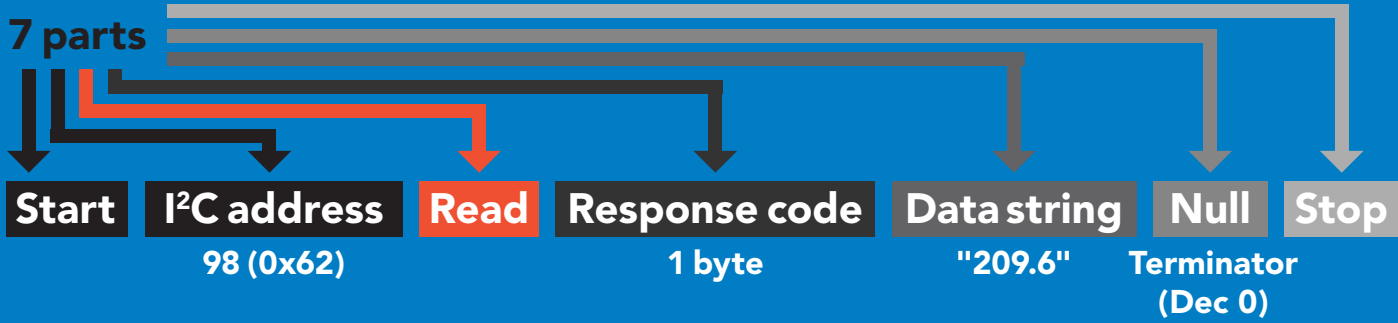

Advanced

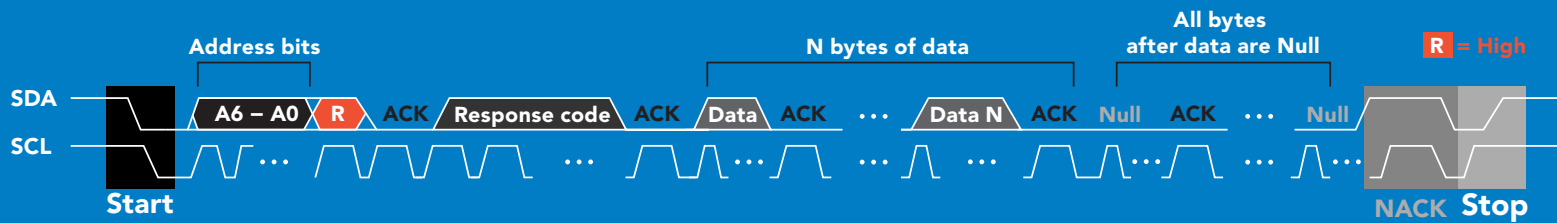


1 50 48 57 46 54 0 = 209.6

Dec ASCII Dec

Response codes

After a command has been issued, a 1 byte response code can be read in order to confirm that the command was processed successfully.

Reading back the response code is completely optional, and is not required for normal operation.

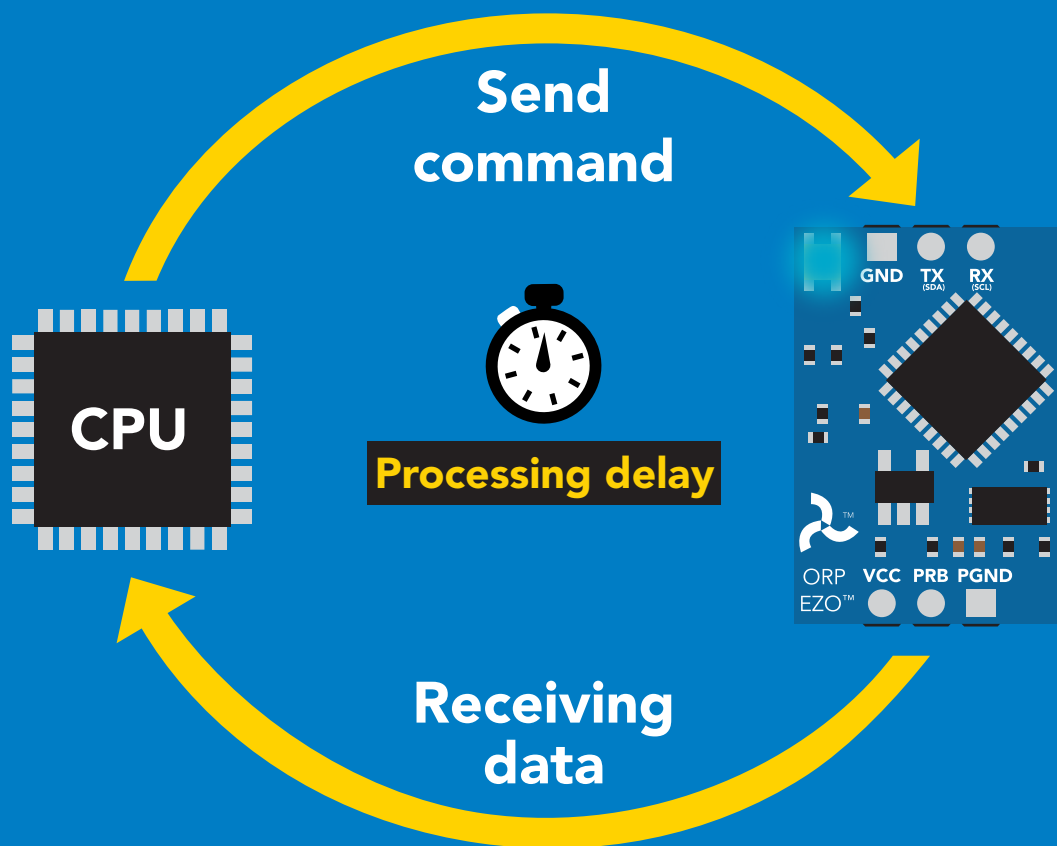

Example

```
I2C_start;  
I2C_address;  
I2C_write(EZO_command);  
I2C_stop;
```

delay(300);



Processing delay

```
I2C_start;  
I2C_address;  
Char[ ] = I2C_read;  
I2C_stop;
```


If there is no processing delay or the processing delay is too short, the response code will always be 254.

Response codes

Single byte, not string


255	no data to send
254	still processing, not ready
2	syntax error
1	successful request

LED color definition

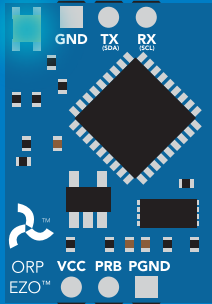


Blue

I²C standby

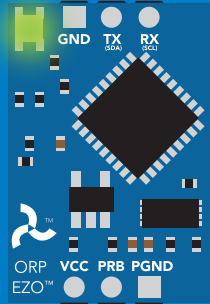


Green

Taking reading

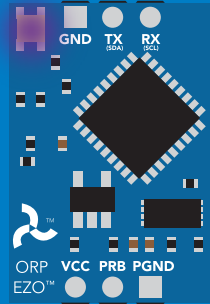


Purple

Changing
I²C ID#

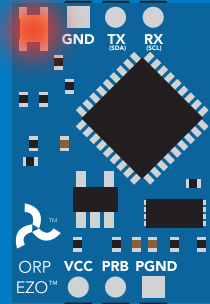

Red

Command
not understood

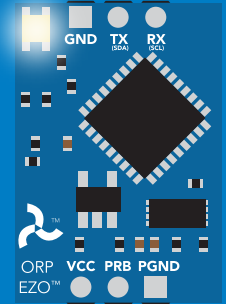

White

Find

5V

LED ON
+2.2 mA

3.3V

+0.6 mA

I²C mode

command quick reference

All commands are ASCII strings or single ASCII characters.

Command	Function	
Baud	switch back to UART mode	pg. 56
Cal	performs calibration	pg. 48
Export/import	export/import calibration	pg. 49
Factory	enable factory reset	pg. 55
Find	finds device with blinking white LED	pg. 46
i	device information	pg. 50
I2C	change I ² C address	pg. 54
L	enable/disable LED	pg. 45
Plock	enable/disable protocol lock	pg. 53
R	returns a single reading	pg. 47
Sleep	enter sleep mode/low power	pg. 52
Status	retrieve status information	pg. 51

LED control

Command syntax

300ms  processing delay

L,1 LED on **default**

L,0 LED off

L,? LED state on/off?

Example

Response

L,1


 **Wait 300ms**
1 Dec 0 Null

L,0


 **Wait 300ms**
1 Dec 0 Null

L,?

 **Wait 300ms**
1 Dec ?L,1 0 Null or 1 Dec ?L,0 0 Null

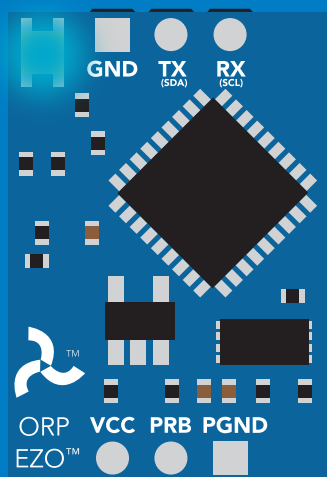

L,1

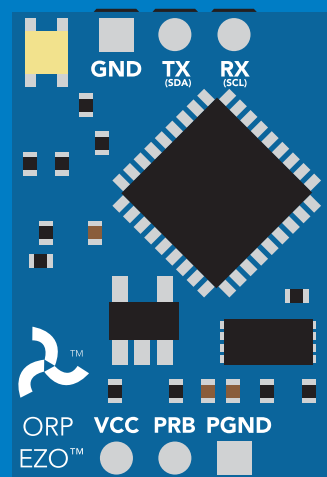

L,0

Find

300ms  processing delay

Command syntax

This command will disable continuous mode
Send any character or command to terminate find.

Find LED rapidly blinks white, used to help find device

Example


Response

Find



1
Dec

0
Null

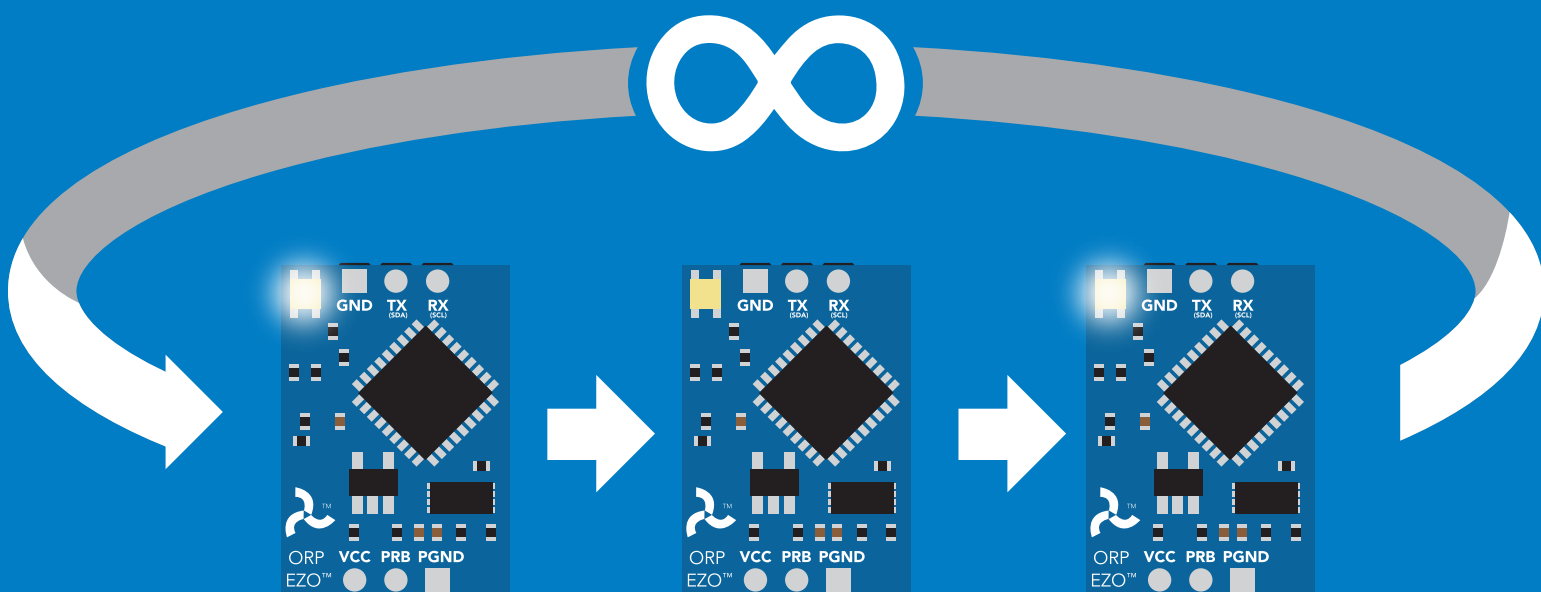

Taking reading

Command syntax

900ms  processing delay


R return 1 reading

Example

R


Response

 **Wait 900ms** **1** **209.6** **0**
Dec ASCII Null

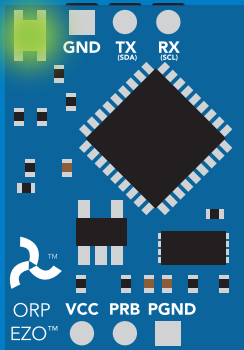


Green



Taking reading



Wait 900ms

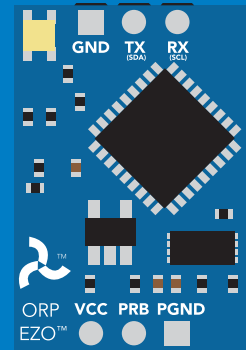

Transmitting

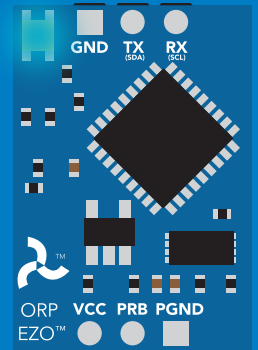

Blue

Standby

Calibration

Command syntax

300ms  processing delay

Cal,n	calibrates the ORP circuit to a set value
Cal,clear	delete calibration data
Cal,?	device calibrated?

The EZO™ ORP circuit can be calibrated to any known ORP value

Example

Response

Cal,225


 Wait 900ms
1 Dec 0 Null

Cal,clear

 Wait 300ms
1 Dec 0 Null

Cal,?

 Wait 300ms
1 Dec ?Cal,0 0 Null or 1 Dec ?Cal,1 0 Null

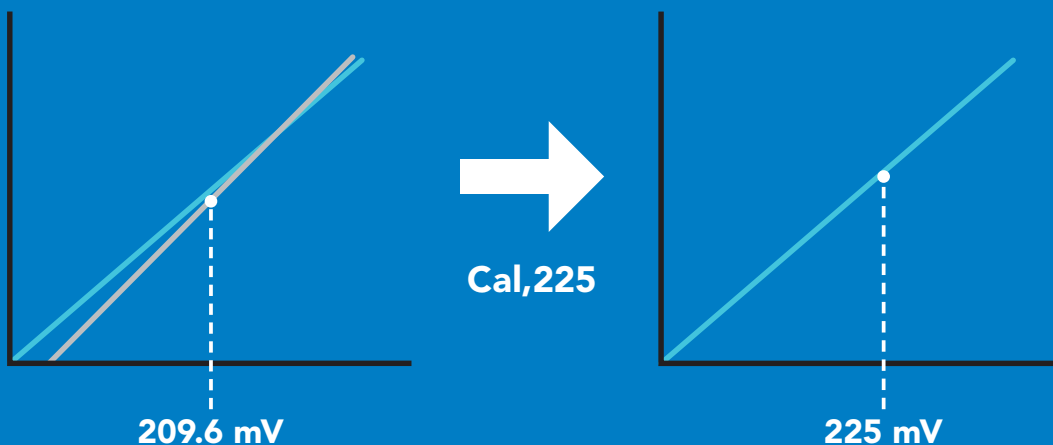

Export/import calibration

Command syntax

Export: Use this command to save calibration settings
Import: Use this command to load calibration settings to one or more devices.

Export	export calibration string from calibrated device
Import	import calibration string to new device
Export,?	calibration string info

300ms  processing delay

Example

Response

Export,?



1

Dec

10,120

ASCII

0

Null

Response breakdown

10, 120

of strings to export

of bytes to export

Export strings can be up to 12 characters long

Export

(8 more)



1

Dec

59 6F 75 20 61 72

ASCII

0

Null

(1 of 10)

⋮

Export



1

Dec

65 20 61 20 63 6F

ASCII

0

Null

(10 of 10)

Export



1

Dec

*DONE

ASCII

0

Null

Import, n
(FIFO)

Import, 59 6F 75 20 61 72

ASCII

(1 of 10)

Device information

Command syntax

300ms  processing delay

i device information

Example

i

Response



Wait 300ms

1

Dec

?i,ORP, 19.7

ASCII

0

Null

Response breakdown

?i, ORP, 1.97
↑ ↑
Device Firmware

Reading device status

Command syntax

300ms  processing delay

Status voltage at Vcc pin and reason for last restart

Example

Response

Status

 **Wait 300ms** **1** **?Status,P,5.038** **0**
Dec ASCII Null

Response breakdown

?Status, **P,** **5.038**
 ↑ ↑
Reason for restart Voltage at Vcc

Restart codes

P	powered off
S	software reset
B	brown out
W	watchdog
U	unknown

Sleep mode/low power

Command syntax

Sleep enter sleep mode/low power

Send any character or command to awaken device.

Example

Response

Sleep


no response

Do not read status byte after issuing sleep command.


Any command

wakes up device

5V	STANDBY	SLEEP
	16 mA	1.16 mA
3.3V	13.9 mA	0.995 mA

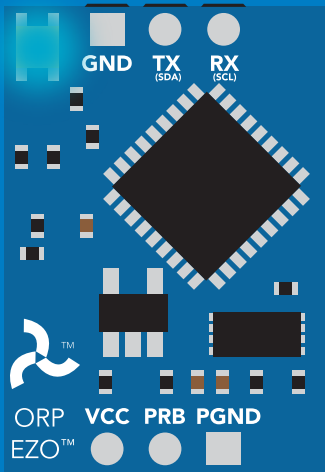

Standby

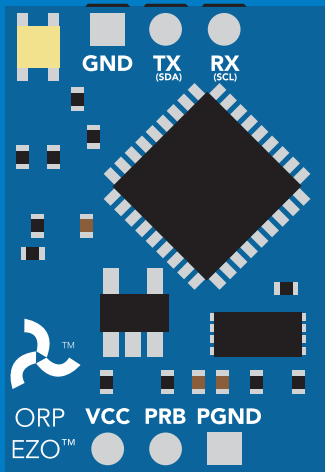

Sleep

Protocol lock

Command syntax

300ms  processing delay

Plock,1 enable Plock

Plock,0 disable Plock

Plock,? Plock on/off?

Locks device to I²C mode.

default

Example

Response

Plock,1

 Wait 300ms
1 Dec 0 Null

Plock,0



 Wait 300ms
1 Dec 0 Null

Plock,?


 Wait 300ms
1 Dec ?Plock,1 0 Null
ASCII

Plock,1

Baud, 9600

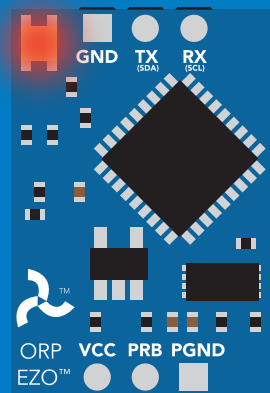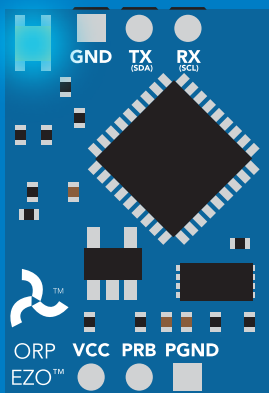

cannot change to UART

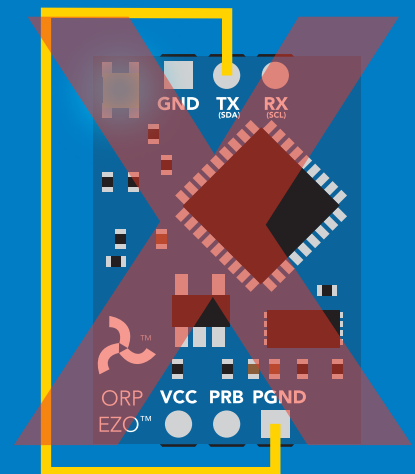

cannot change to UART

I²C address change

Command syntax

300ms  processing delay

I2C,n sets I²C address and reboots into I²C mode

Example

Response

I2C,100

device reboot


Warning!

Changing the I²C address will prevent communication between the circuit and the CPU, until the CPU is updated with the new I²C address.


Default I²C address is 98 (0x62).

n = any number 1 – 127

I2C,100

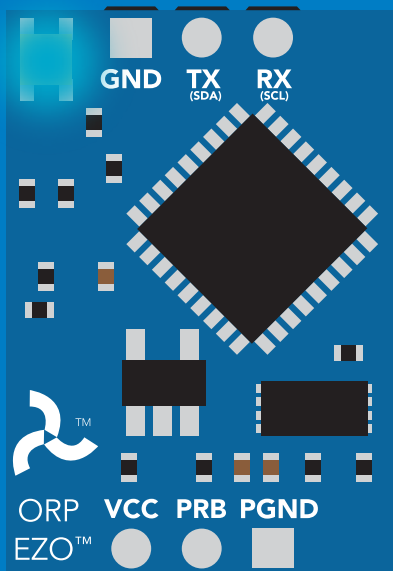

(reboot)

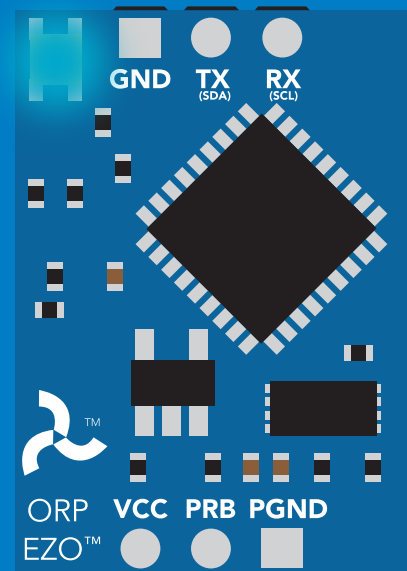

Factory reset

Command syntax

Factory reset will not take the device out of I²C mode.

Factory enable factory reset

I²C address will not change

Example



Factory

Response


device reboot

Clears calibration
LED on
Response codes enabled

Factory

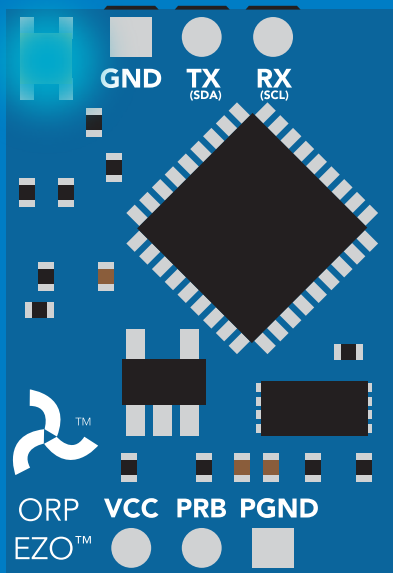

(reboot)

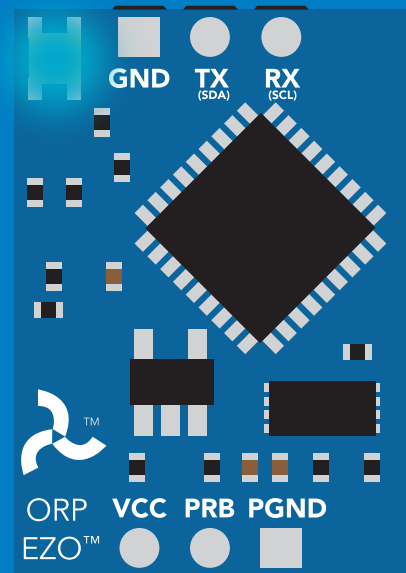

Change to UART mode

Command syntax

Baud,n switch from I²C to UART

Example



Baud,9600

Response


reboot in UART mode

n =


- 300
- 1200
- 2400
- 9600
- 19200
- 38400
- 57600
- 115200

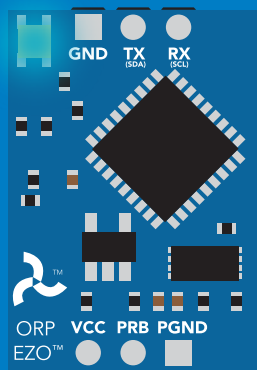


Baud,9600

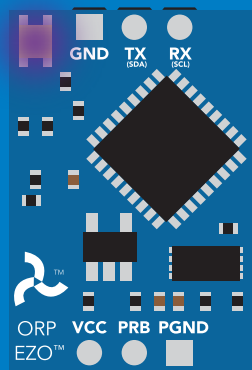

Changing to
UART mode




(reboot)

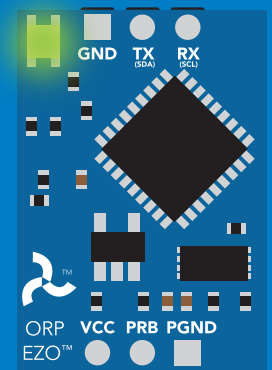


Manual switching to UART

- Make sure Plock is set to 0
- Disconnect ground (power off)
- Disconnect TX and RX
- Connect TX to PGND
- Confirm RX is disconnected
- Connect ground (power on)
- Wait for LED to change from Blue to Green
- Disconnect ground (power off)
- Reconnect all data and power


Example

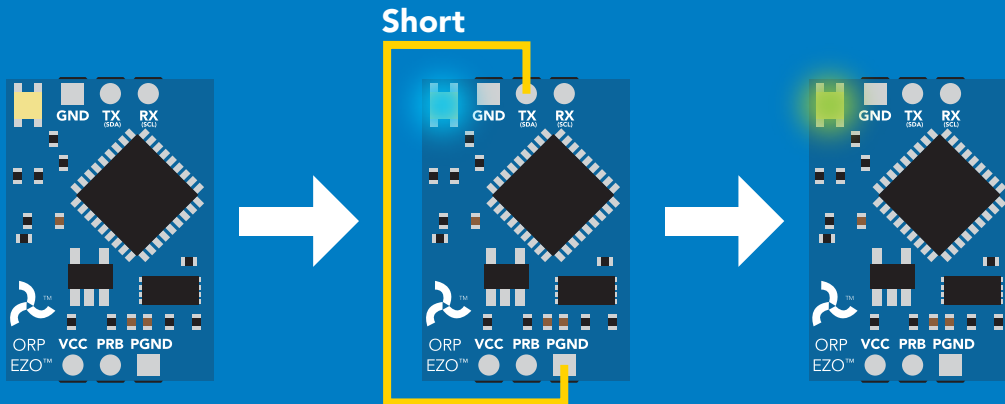

Wrong Example

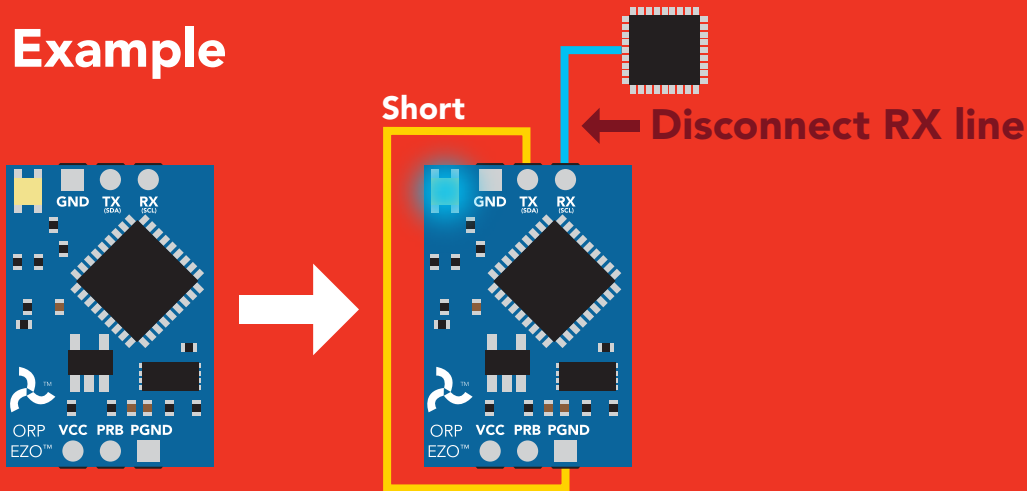


EZO™ circuit footprint

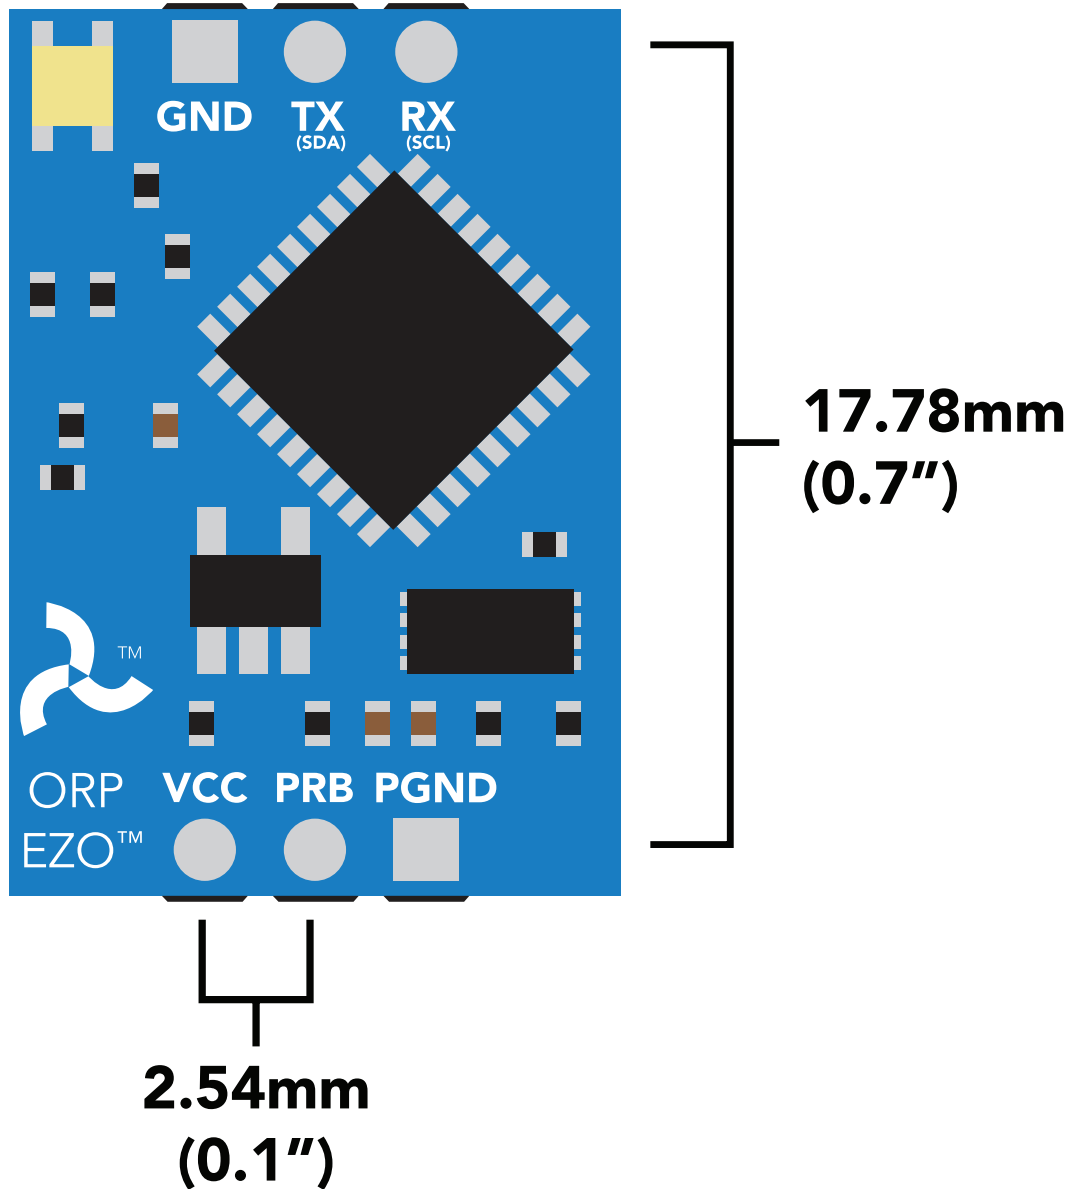


1 In your CAD software place an 8 position header.



2 Place a 3 position header at both top and bottom of the 8 position.

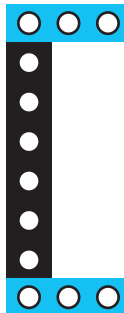

3 Delete the 8 position header. The two 3 position headers are now 17.78mm (0.7") apart from each other.

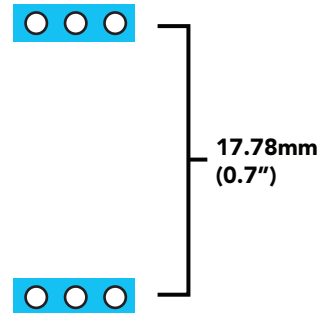

Datasheet change log

Datasheet V 4.2

Removed note from certain commands about firmware version.

Datasheet V 4.1

Added information to calibration theory on pg 8.

Datasheet V 4.0

Revised definition of response codes on pg 42.

Datasheet V 3.9

Revised isolation information on pg 9.

Datasheet V 3.8

Revised Plock pages to show default value.

Datasheet V 3.7

Added new commands:

"Find" pages 23 (UART) & 46 (I²C).

"Export/Import calibration" pages 27 (UART) & 49 (I²C).

Added new feature to continous mode "C,n" pg 24.

Datasheet V 3.6

Revised circuit illustrations throughout datasheet.

Datasheet V 3.5

Added accuracy range on cover page, and revised isolation info on pg 10.

Datasheet V 3.4

Revised entire datasheet.

Firmware updates

V1.5 – Baud rate change (Nov 6, 2014)

- Change default baud rate to 9600

V1.6 – I²C bug (Dec 1, 2014)

- Fixed I²C bug where the circuit may inappropriately respond when other I²C devices are connected.

V1.7 – Factory (April 14, 2015)

- Changed "X" command to "Factory"

V1.95 – Plock (March 31, 2016)

- Added protocol lock feature "Plock"

V1.96 – EEPROM (April 26, 2016)

- Fixed glitch where EEPROM would get erased if the circuit lost power 900ms into startup

V1.97 – EEPROM (Oct 10, 2016)

- Fixed glitch in the cal clear command, improves how it calculates the ORP
- Added calibration saving and loading

V2.10 – (May 9, 2017)

- Added "Find" command.
- Added "Export/import" command.
- Modified continuous mode to be able to send readings every "n" seconds.

Warranty

Atlas Scientific™ Warranties the EZO™ class ORP circuit to be free of defect during the debugging phase of device implementation, or 30 days after receiving the EZO™ class ORP circuit (which ever comes first).

The debugging phase

The debugging phase as defined by Atlas Scientific™ is the time period when the EZO™ class ORP circuit is inserted into a bread board, or shield. If the EZO™ class ORP circuit is being debugged in a bread board, the bread board must be devoid of other components. If the EZO™ class ORP circuit is being connected to a microcontroller, the microcontroller must be running code that has been designed to drive the EZO™ class ORP circuit exclusively and output the EZO™ class ORP circuit data as a serial string.

It is important for the embedded systems engineer to keep in mind that the following activities will void the EZO™ class ORP circuit warranty:

- Soldering any part of the EZO™ class ORP circuit.
- Running any code, that does not exclusively drive the EZO™ class ORP circuit and output its data in a serial string.
- Embedding the EZO™ class ORP circuit into a custom made device.
- Removing any potting compound.

Reasoning behind this warranty

Because Atlas Scientific™ does not sell consumer electronics; once the device has been embedded into a custom made system, Atlas Scientific™ cannot possibly warranty the EZO™ class ORP circuit, against the thousands of possible variables that may cause the EZO™ class ORP circuit to no longer function properly.

Please keep this in mind:

- 1. All Atlas Scientific™ devices have been designed to be embedded into a custom made system by you, the embedded systems engineer.**
- 2. All Atlas Scientific™ devices have been designed to run indefinitely without failure in the field.**
- 3. All Atlas Scientific™ devices can be soldered into place, however you do so at your own risk.**

Atlas Scientific™ is simply stating that once the device is being used in your application, Atlas Scientific™ can no longer take responsibility for the EZO™ class ORP circuits continued operation. This is because that would be equivalent to Atlas Scientific™ taking responsibility over the correct operation of your entire device.